

High Performance Liquid Chromatography

Analysis Information

Product Name: BIM, Biotinylated

Operator: David

Injection Date: 1/19/2022 2:02:07 PM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
10.0min	Stop	Stop

Flow rate: 0.45ml/min

Wavelength: 210nm

Volume: 3 μ l

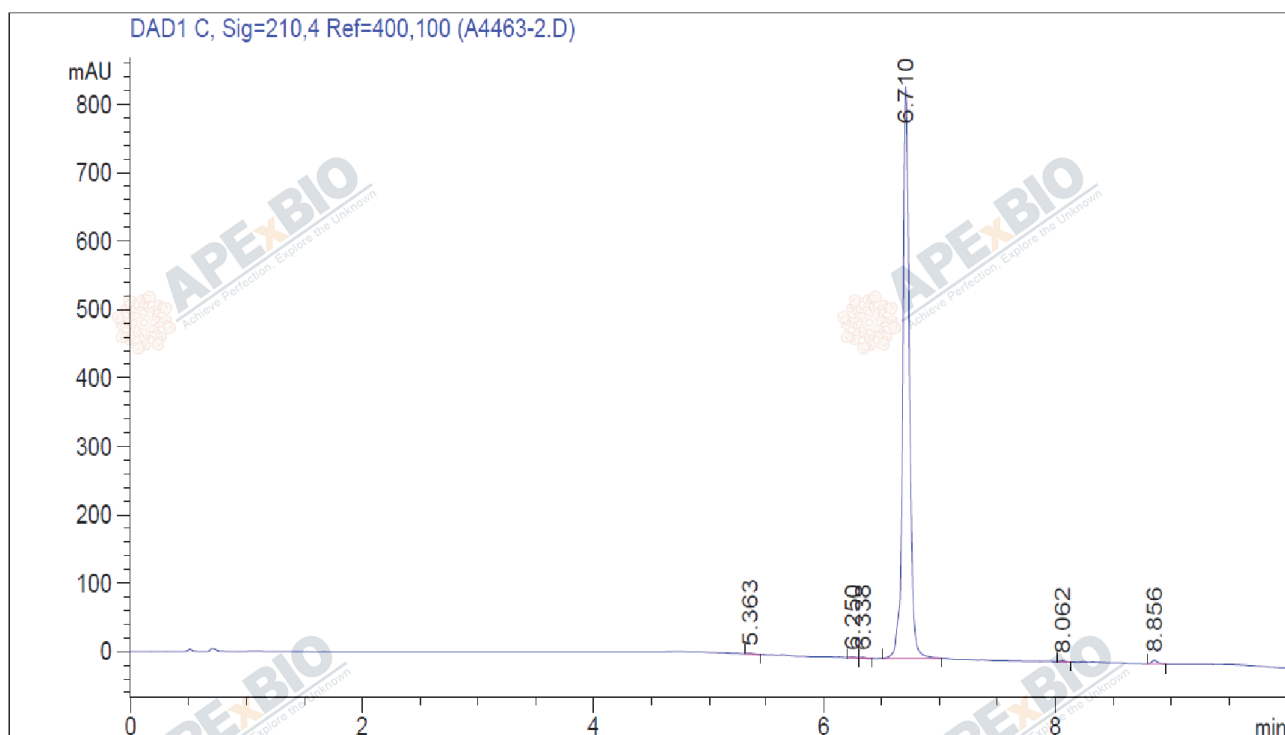

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.363	3.88130	0.1150
2	6.250	3.56538	0.1056
3	6.338	3.46667	0.1027
4	6.710	3342.71387	99.0418
5	8.062	3.31484	0.0982
6	8.856	18.11232	0.5367

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com

