

High Performance Liquid Chromatography

Analysis Information

Product Name: IBT6A

Operator: David

Injection Date: 2023-11-29 16:03:45+08:00

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	95%	5%
2.0min	95%	5%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 2 μ l

Result

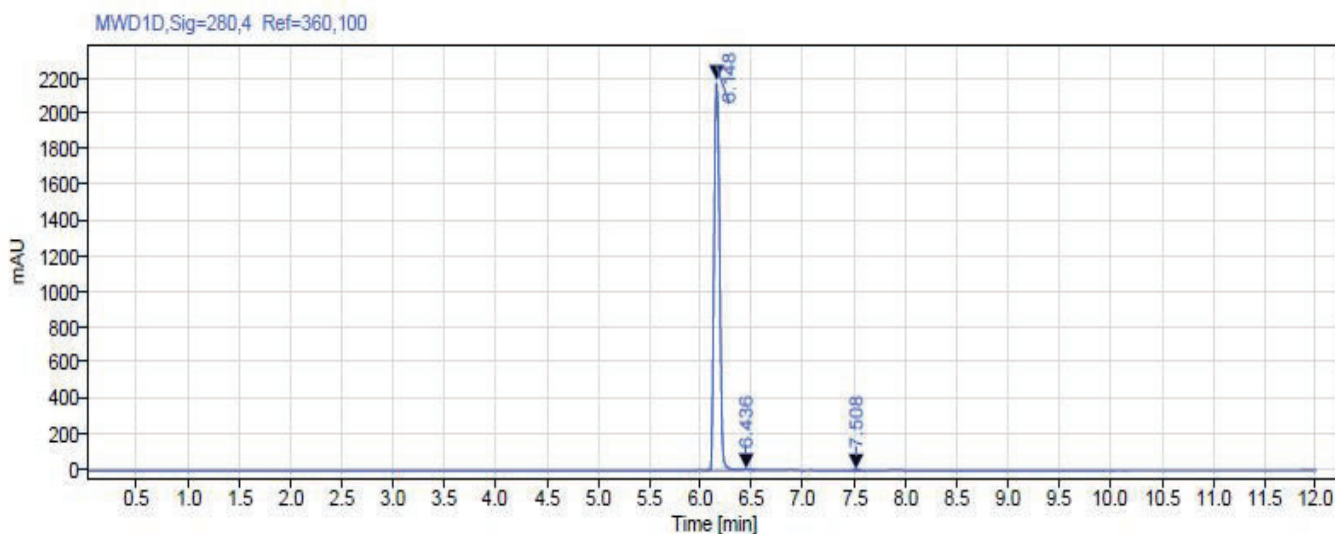

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.148	8207.58	99.43
2	6.436	31.32	0.38
3	7.508	15.41	0.19

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com