

Mass Spectrometry

Analysis Information

Product Name: EDC.HCl

Operator: David

Injection Date: 8/26/2020 9:31:34 AM

Inj. Volume: 1

Batch No.: 4

Acquisition Parameter

Probe: ESI

Gas Temp: 350°C

Gas Flow: 11L/min

Nebulizer: 50psi

VCap: 4000v

Fragmentor: 70v

Reference: m/z 121.050873, 922.009798

T.Flow: 0.3ml/min


B.conc: 20%H₂O/80%ACN

Result

NT-S20200826-014

20200826-A7021-4 8 (0.130)

1: Scan ES+
8.90e7

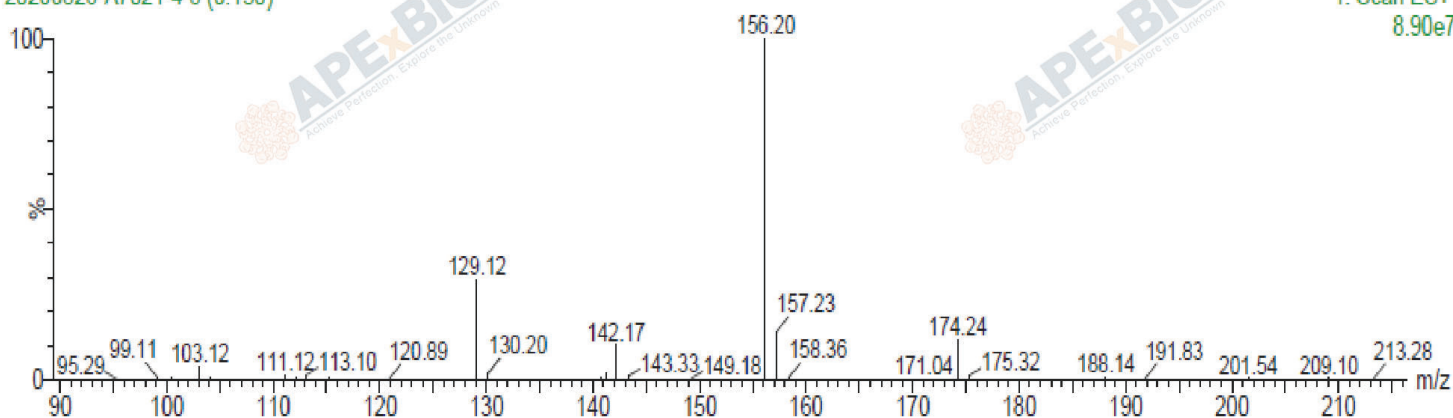

Molecular Weight: 191.7

m/z([M-HCl]-) Base Peak: 156.20

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com