

High Performance Liquid Chromatography

Analysis Information

Product Name: HOAt

Operator: David

Injection Date: 5/25/2022 7:05:37 PM

Batch No.: 14

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA

Gradient:


Time	A	B
0.0min	10%	90%
5.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 254nm

Volume: 4 μ l

Result

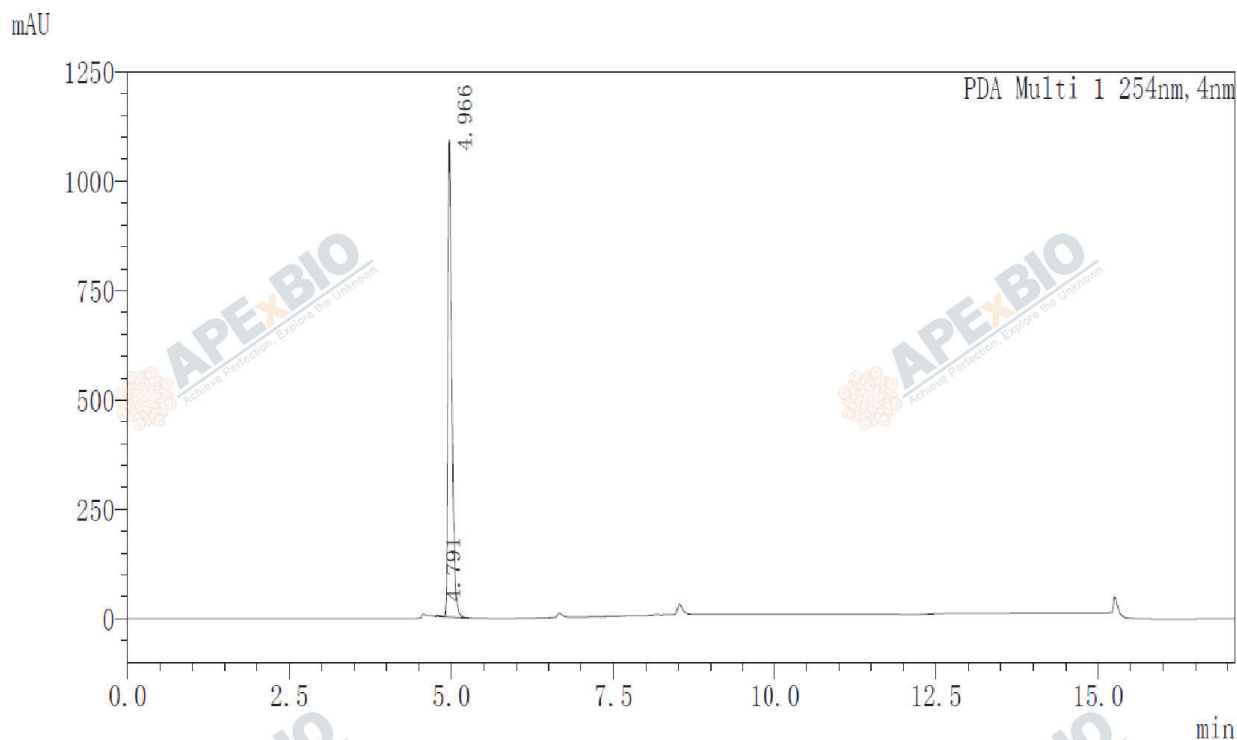

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.791	6840	0.149
2	4.966	4588071	99.851

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com