

High Performance Liquid Chromatography

Analysis Information

Product Name: HOBt

Operator: David

Injection Date: 1/19/2022 3:22:52 PM

Batch No.: 18

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
10.0min	Stop	Stop

Flow rate: 0.45ml/min

Wavelength: 210nm

Volume: 3 μ l

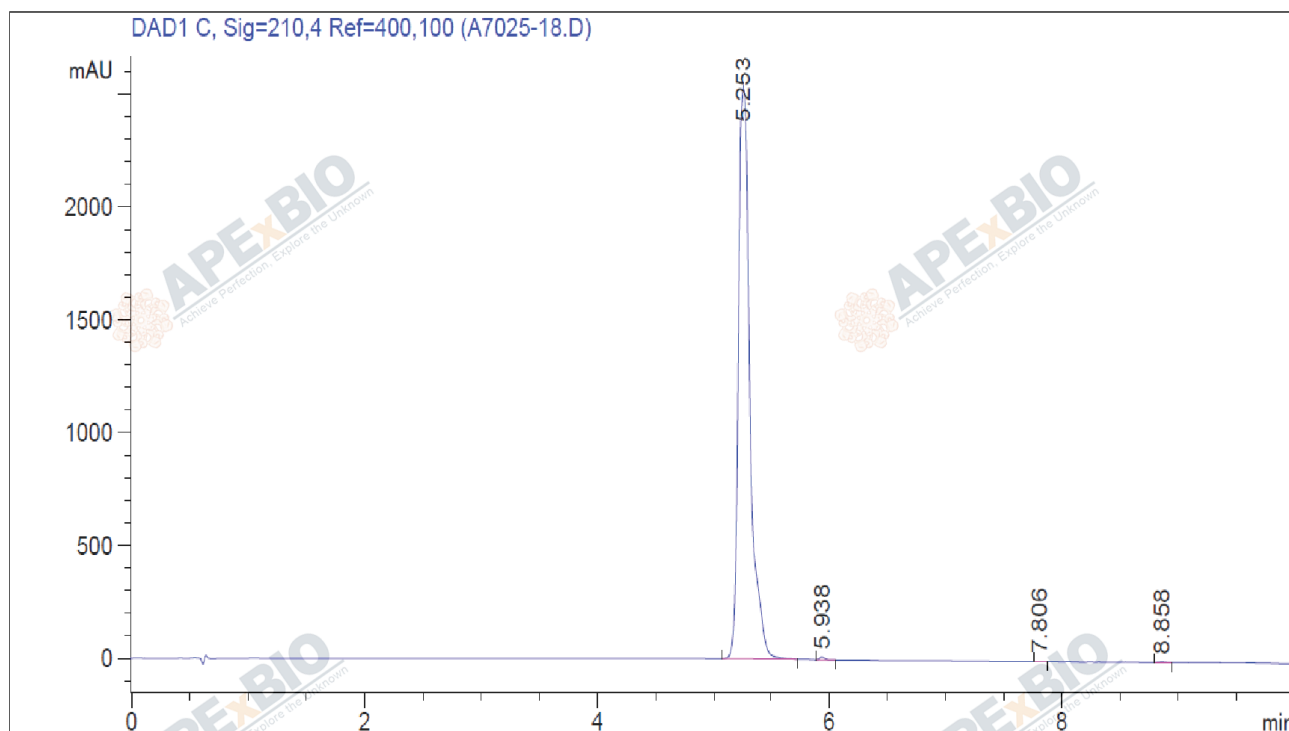

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.253	1.93694e4	99.7414
2	5.938	35.03446	0.1804
3	7.806	3.98284	0.0205
4	8.858	11.19984	0.0577

Caution**FOR RESEARCH PURPOSES ONLY.****NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.****APExBIO Technology****www.apexbt.com**

7505 Fannin street, Suite 410, Houston, TX 77054.

