

High Performance Liquid Chromatography

Analysis Information

Product Name: HOBt

Operator: David

Injection Date: 2/21/2022 5:44:46 PM

Batch No.: 19

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
10.0min	Stop	Stop

Flow rate: 0.45ml/min

Wavelength: 210nm

Volume: 3 μ l

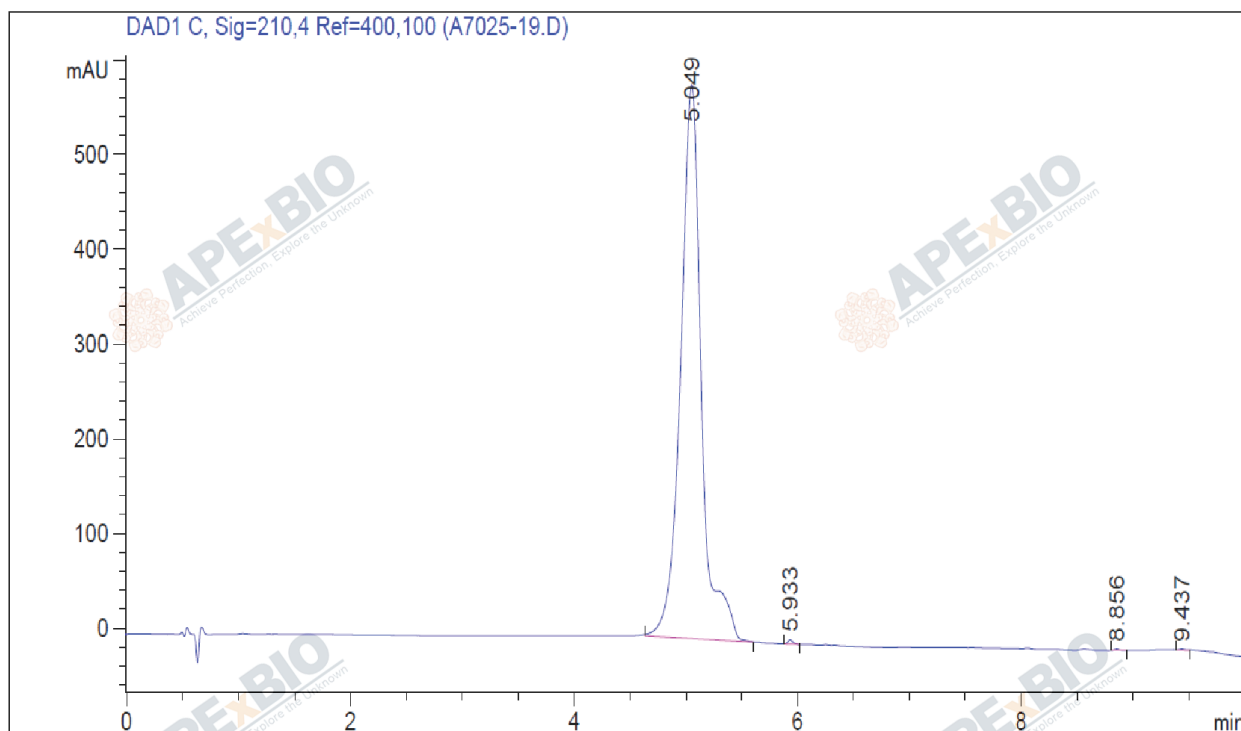

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.049	7502.98486	99.6773
2	5.933	13.53127	0.1798
3	8.856	5.10231	0.0678
4	9.437	5.65793	0.0752

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

