

## 1. Analysis Information

Product Name:	NHS-SS-Biotin
Operator:	David
Injection Date:	6/12/2018 14:42:03 PM
Inj. Volume:	1
Batch No.:	8


## 2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H <sub>2</sub> O/80%ACN

## 3. Result

20180612-B1-0608 9 (0.156)

2: Scan ES-  
2.10e7

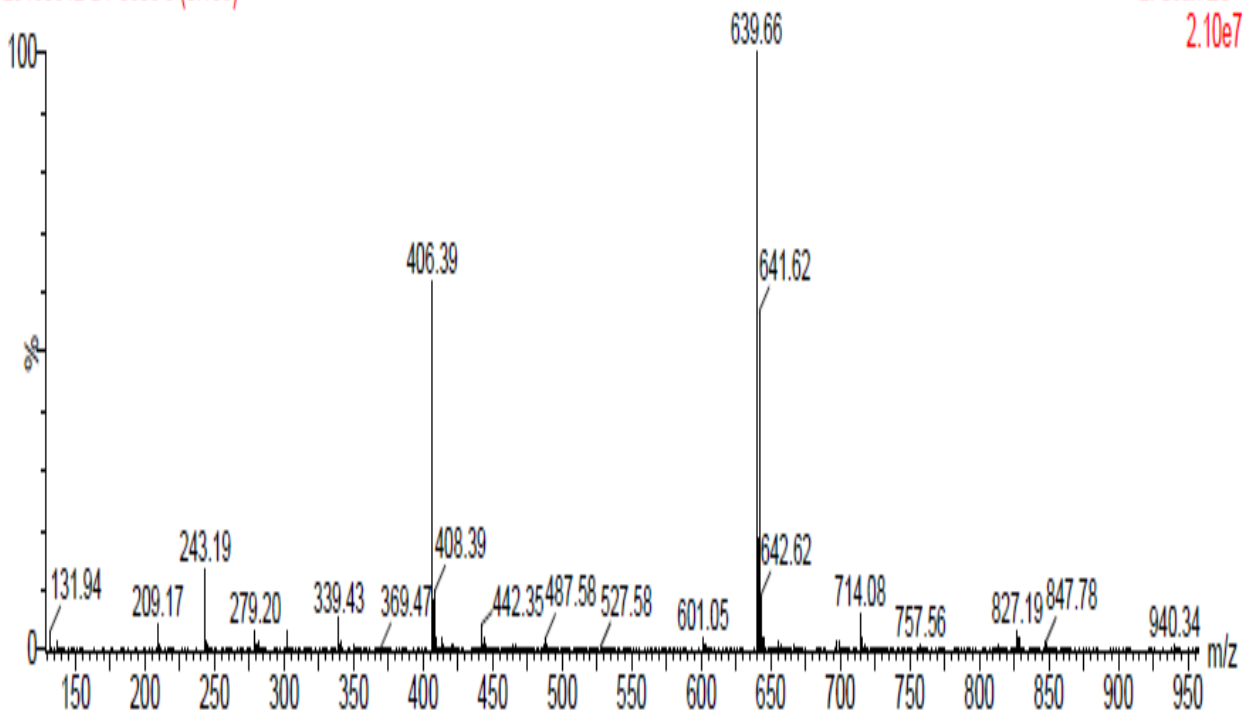

Molecular Weight:	504.64
m/z([M+C <sub>4</sub> H <sub>4</sub> NO <sub>2</sub> +Cl] <sup>+</sup> )Base Peak :	639.66
m/z([M-C <sub>4</sub> H <sub>4</sub> NO <sub>2</sub> -H] <sup>-</sup> )Base Peak :	406.39