


7.361
7.345
7.338
7.331
7.309
7.300
7.276
7.270
7.249
7.199
7.178
6.487
6.469
5.352
5.333
5.093
4.966
4.963
4.809
4.806
4.780
4.773
4.756
4.750
4.733
4.726
4.454
4.430
3.155
3.132
3.108
3.086
3.070
3.047
3.025
3.001
1.314
1.290

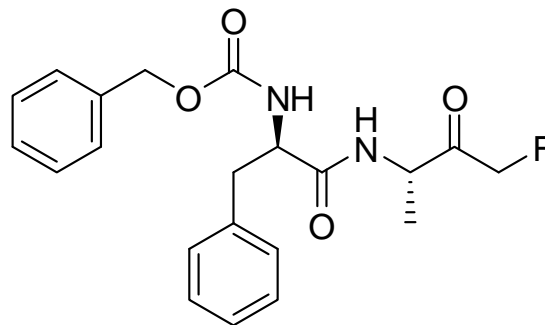


```

NAME          Z-FA-FMK
EXPNO         1
PROCNO        1
Date_         20130613
Time_         14.57
INSTRUM       spect
PROBHD        5 mm PABBO BB-
PULPROG       zg30
TD            32768
SOLVENT       CDCl3
NS            8
DS            2
SWH           6009.615 Hz
FIDRES        0.183399 Hz
AQ            2.7263477 sec
RG            181
DW            83.200 usec
DE            6.50 usec
TE            298.0 K
D1            1.00000000 sec
TD0           1
  
```

```

===== CHANNEL f1 =====
SFO1          300.1324010 MHz
NUC1           1H
P1            12.90 usec
SI            65536
SF            300.1300061 MHz
WDW           EM
SSB           0
LB            0.30 Hz
GB            0
PC            1.00
  
```

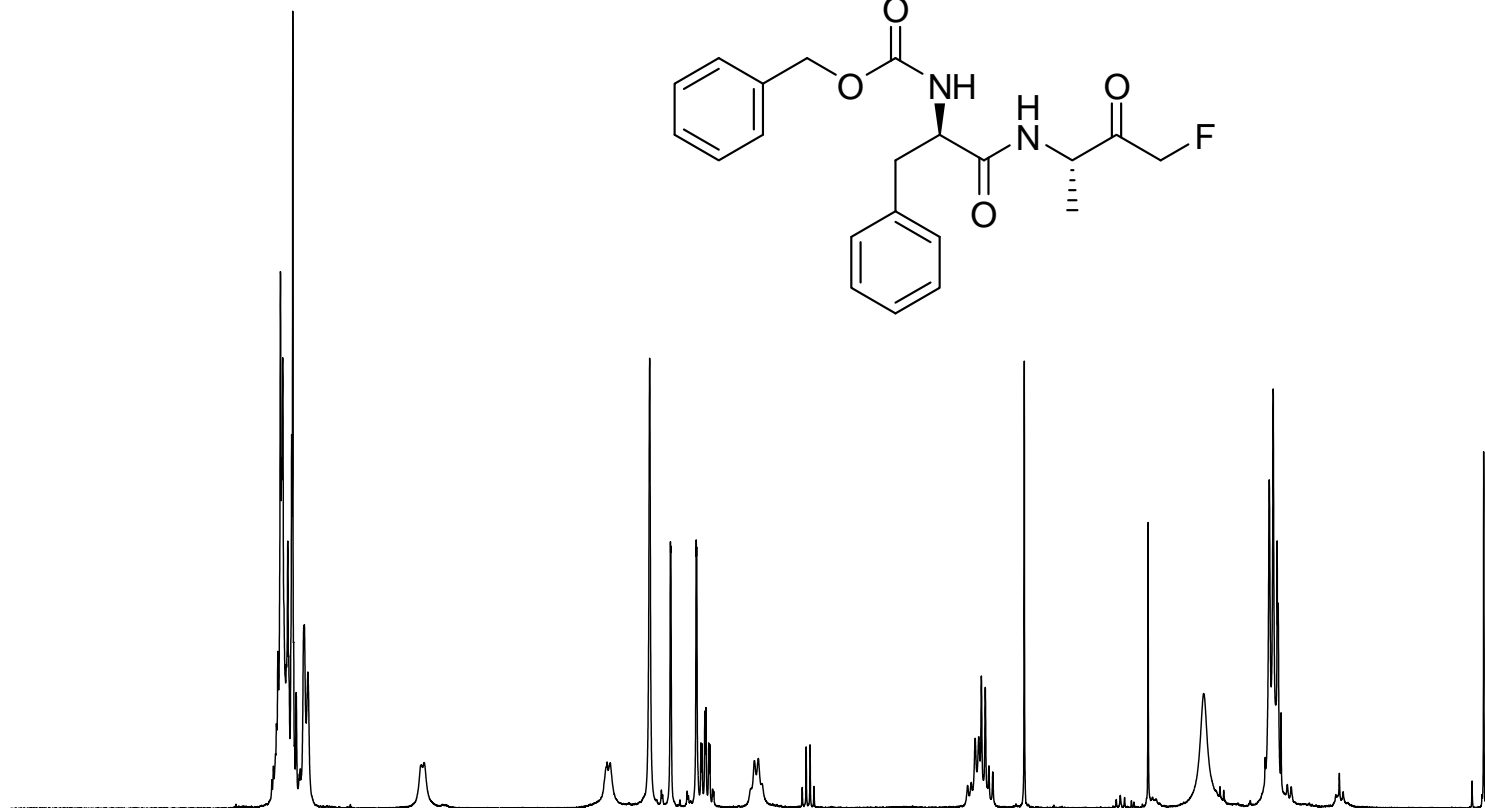

8.5 8.0 7.5 7.0 6.5 6.0 5.5 5.0 4.5 4.0 3.5 3.0 2.5 2.0 1.5 1.0 ppm

7.23
2.88
0.93
0.96
2.00
0.94
1.01
0.93
1.04
2.21
3.37