

# Mass Spectrometry


## 1. Analysis Information

Product Name:	Entinostat (MS-275,SNDX-275)
Operator:	David
Injection Date:	8/15/2013 04:19:02 PM
Inj. Volume:	1
Batch No.:	2

## 2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	150v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20% H <sub>2</sub> O/80% ACN

## 3. Result

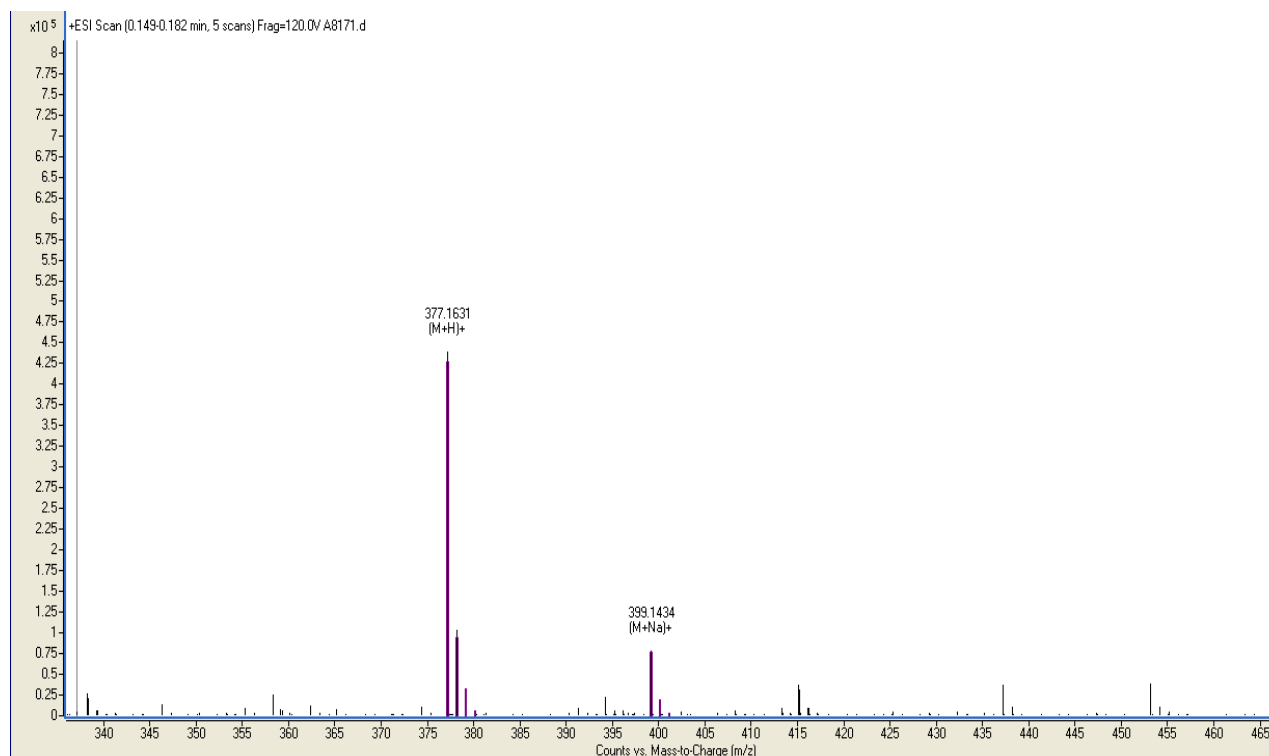

Molecular Weight:	376.40
m/z(M+H) Base Peak :	377.1631
m/z(M+Na) Base Peak :	399.1434