



High Performance Liquid Chromatography


1. Analysis Information

Product Name:	GDC-0941
Operator:	David
Injection Date:	11/25/2013 10:59:25 AM
Batch No.:	1

2. HPLC Condition

Column:	Venusil XBridge C18 ,4.6*150mm, 3.5um,300A																
Solvent A:	0.1% Trifluoroacetic in 100% Acetonitrile																
Solvent B:	0.1% Trifluoroacetic in 100% Water																
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>95%</td><td>5%</td></tr><tr><td>3.0min</td><td>95%</td><td>5%</td></tr><tr><td>6.0min</td><td>95%</td><td>5%</td></tr><tr><td>6.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	95%	5%	3.0min	95%	5%	6.0min	95%	5%	6.0min	Stop	Stop
Time	A	B															
0.0min	95%	5%															
3.0min	95%	5%															
6.0min	95%	5%															
6.0min	Stop	Stop															
Flow rate:	1.0ml/min																
Wavelength:	254nm																
Volume:	10µl																

3. Result

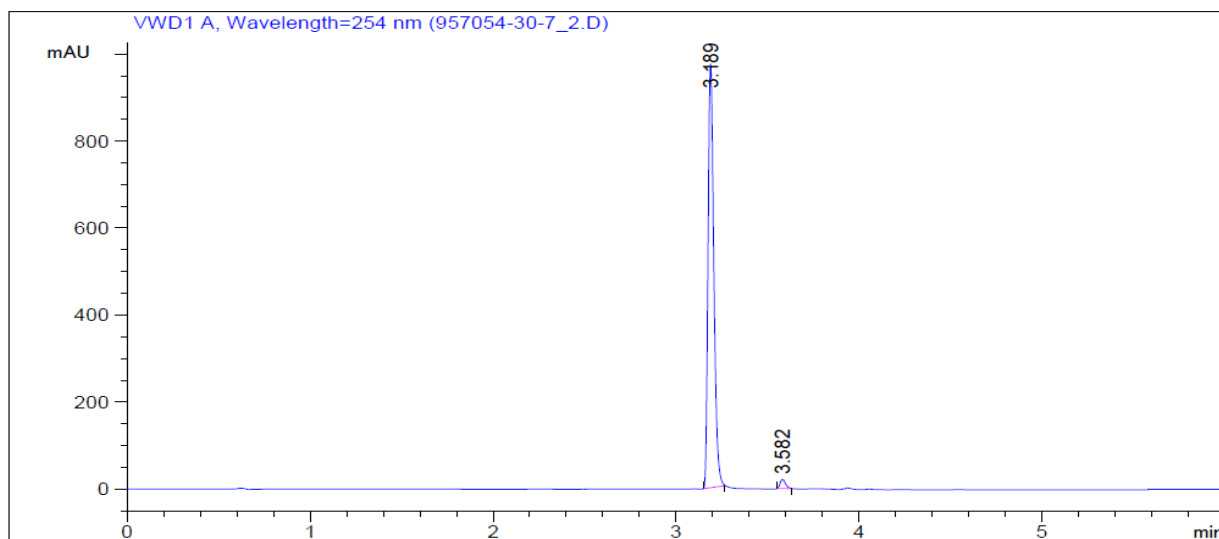

Rank	RetTime(min)	Area(mAU*s)	Area %
1	3.189	2132.25977	98.0630
2	3.582	42.11800	1.9370