

High Performance Liquid Chromatography

Analysis Information

Product Name: VX-765

Operator: David

Injection Date: 2/16/2022 11:39:09 AM

Batch No.: 3

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
10.0min	Stop	Stop

Flow rate: 0.45ml/min

Wavelength: 210nm

Volume: 3 μ l

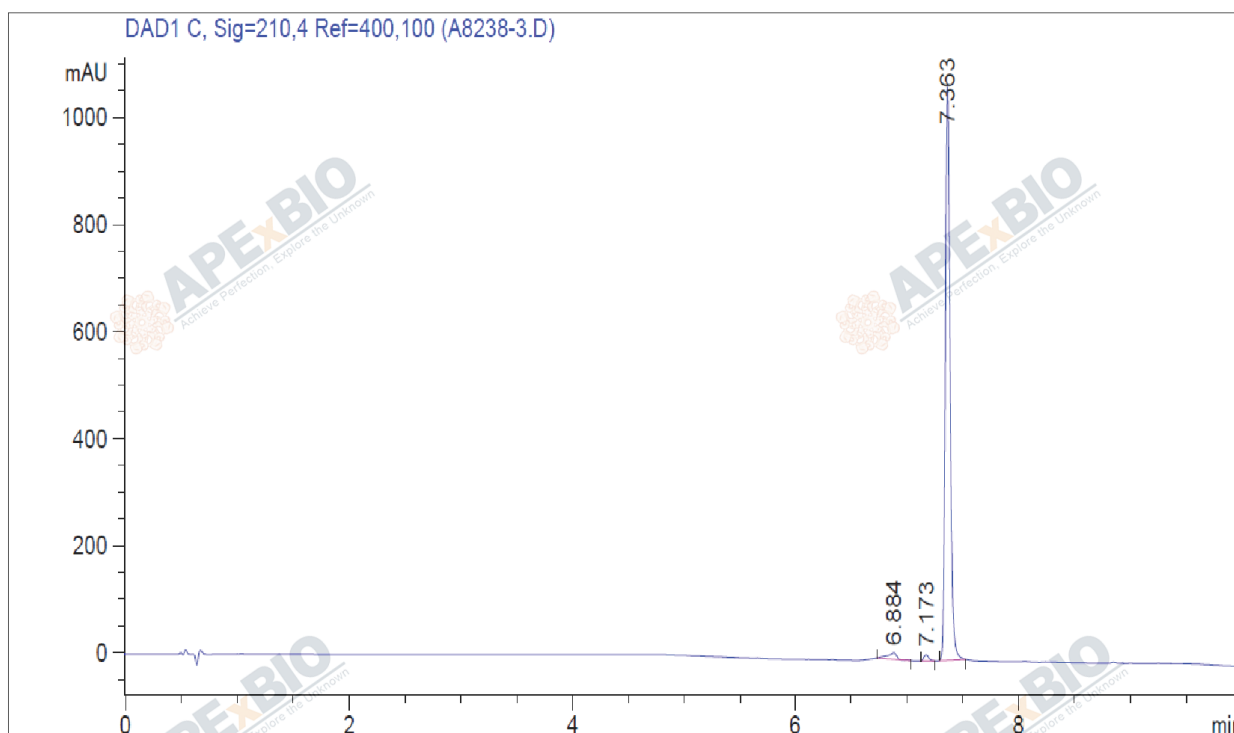

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.884	68.56722	2.0773
2	7.173	32.64243	0.9889
3	7.363	3199.57202	96.9338

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com