

## 1. Analysis Information

Product Name:	CHIR-99021 (CT99021) HCl
Operator:	David
Injection Date:	4/29/2016 01:22:18 PM
Inj. Volume:	1
Batch No.:	2


## 2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H <sub>2</sub> O/80%ACN

## 3. Result

20160901-11-0830 29 (0.504)

2: Scan ES-  
1.12e6

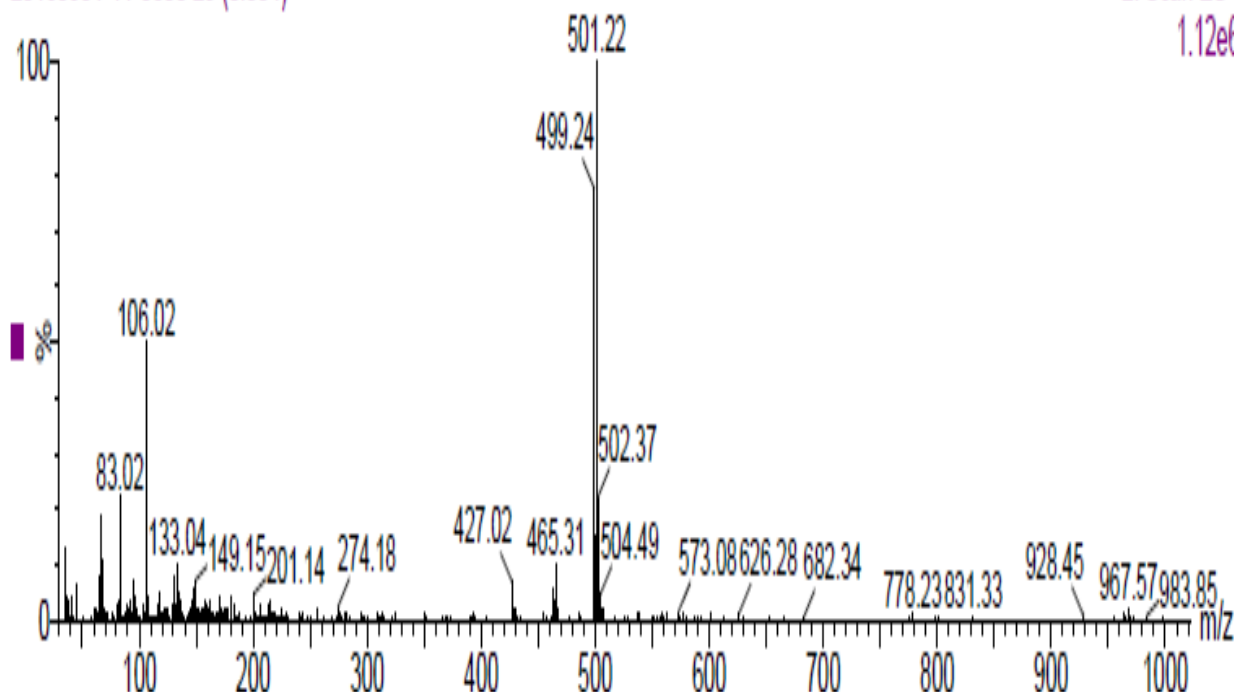

Molecular Weight:	501.8
m/z(M-2H) Base Peak :	502.37
m/z(M-H) Base Peak :	504.49