

High Performance Liquid Chromatography

Analysis Information

Product Name: ITE

Operator: David

Injection Date: 12/2/2021 12:51:14 PM

Batch No.: 4

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA

Gradient:


Time	A	B
0.0min	10%	90%
5.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 358nm

Volume: 3 μ l

Result

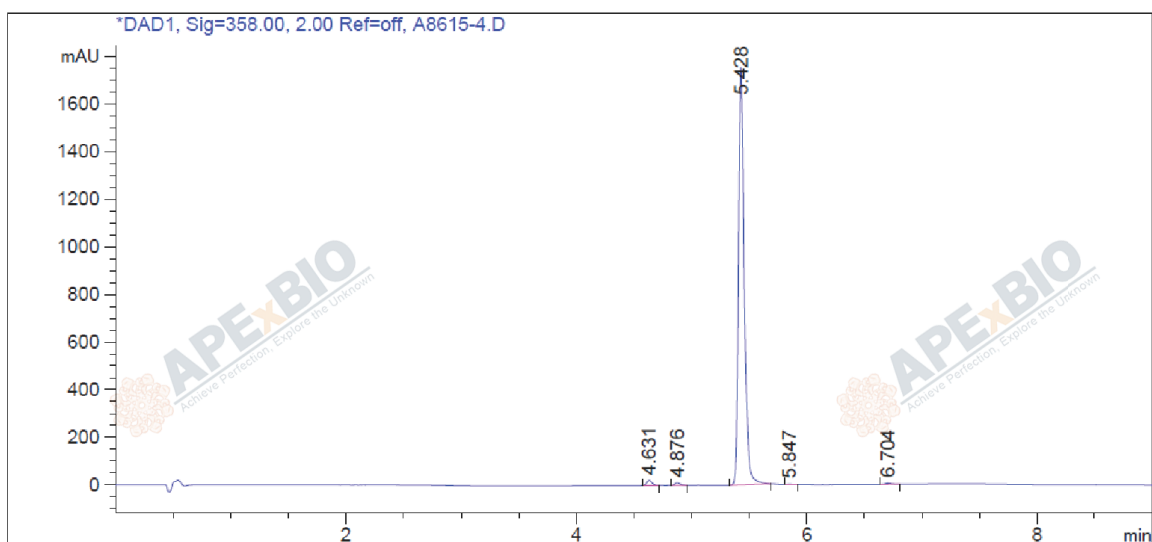

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.631	70.65603	1.1253
2	4.876	34.30705	0.5464
3	5.428	6155.30029	98.0319
4	5.847	3.30583	0.0526
5	6.704	15.30853	0.2438

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com