

High Performance Liquid Chromatography

Analysis Information

Product Name: ITE

Operator: David

Injection Date: 3/14/2022 11:53:28 AM

Batch No.: 6

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 360nm

Volume: 3 μ l

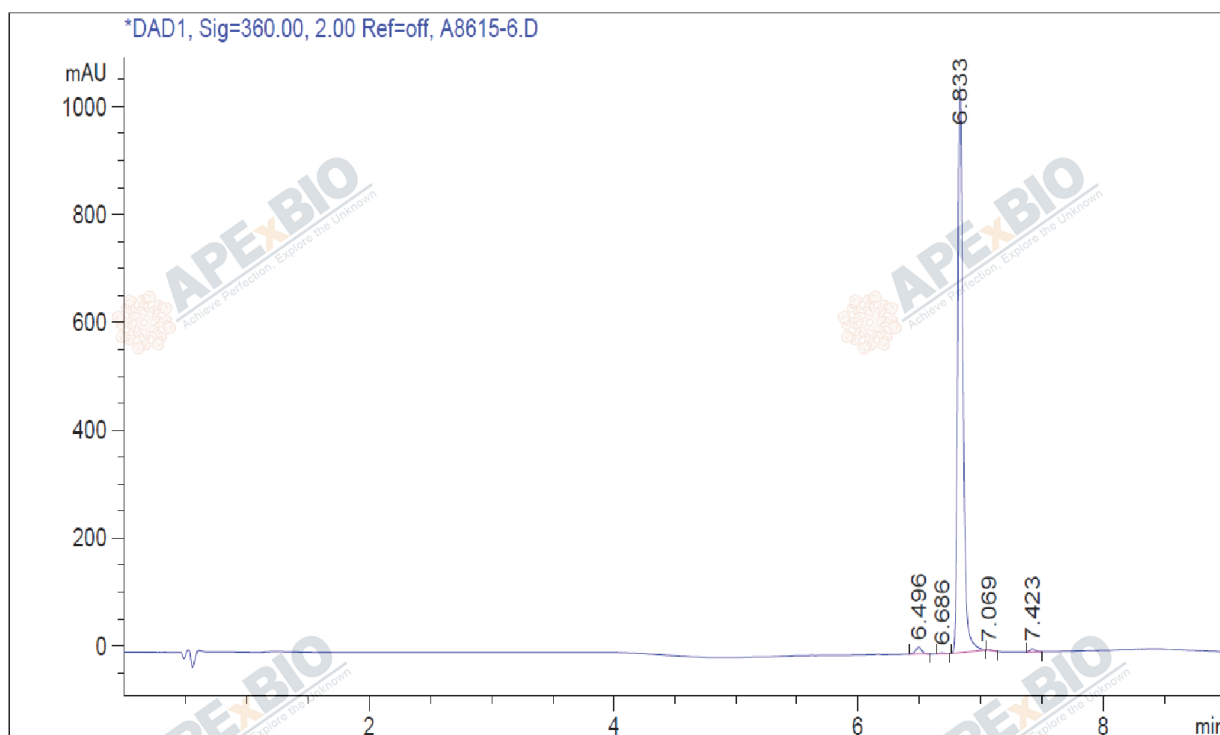

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.496	42.07948	1.2998
2	6.686	4.18500	0.1293
3	6.833	3172.89746	98.0053
4	7.069	3.64209	0.1125
5	7.423	14.67074	0.4532

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com

