



# High Performance Liquid Chromatography


## 1. Analysis Information

Product Name:	MYK-461
Operator:	David
Injection Date:	11/10/2016 6:35:29 PM
Batch No.:	1

## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm																
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																
Solvent B:	0.1% H3PO4 in 100% Water																
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>5%</td><td>95%</td></tr><tr><td>9.0min</td><td>5%</td><td>95%</td></tr><tr><td>15.0min</td><td>95%</td><td>5%</td></tr><tr><td>15.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	5%	95%	9.0min	5%	95%	15.0min	95%	5%	15.0min	Stop	Stop
Time	A	B															
0.0min	5%	95%															
9.0min	5%	95%															
15.0min	95%	5%															
15.0min	Stop	Stop															
Flow rate:	0.4ml/min																
Wavelength:	210nm																
Volume:	10 $\mu$ l																

## 3. Result

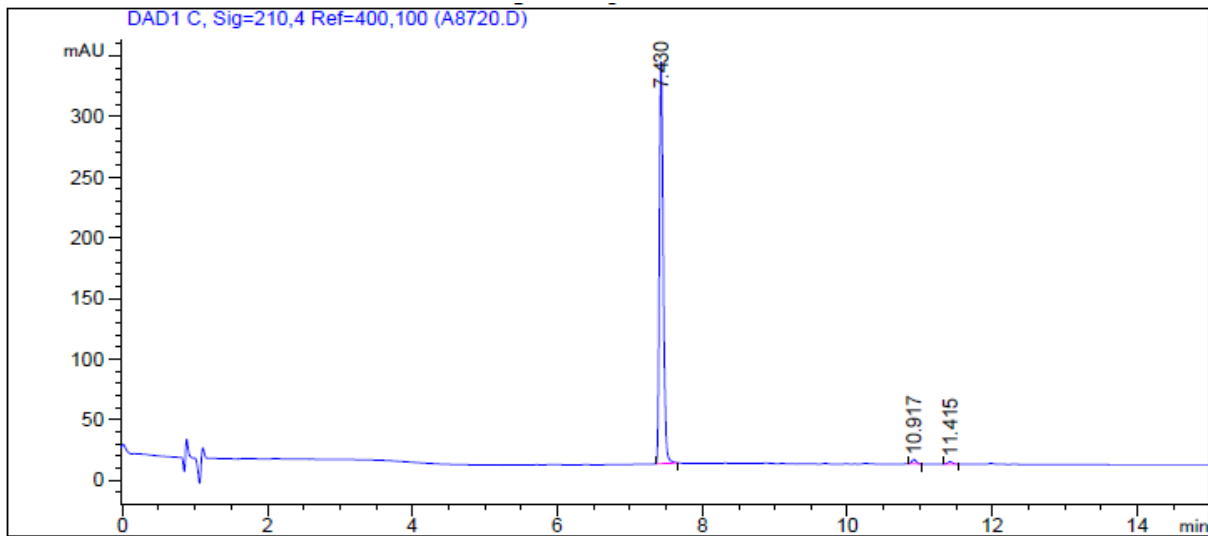

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.430	1238.73218	98.1474
2	10.917	14.92842	1.1828
3	11.415	8.45328	0.6698