

## 1. Analysis Information

Product Name:	C598-0466
Operator:	David
Injection Date:	3/20/2017 2:17:00 PM
Inj. Volume:	1
Batch No.:	1


## 2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H <sub>2</sub> O/80%ACN

## 3. Result

20170320-B1-0315 11 (0.182)

1: Scan ES+  
6.22e7

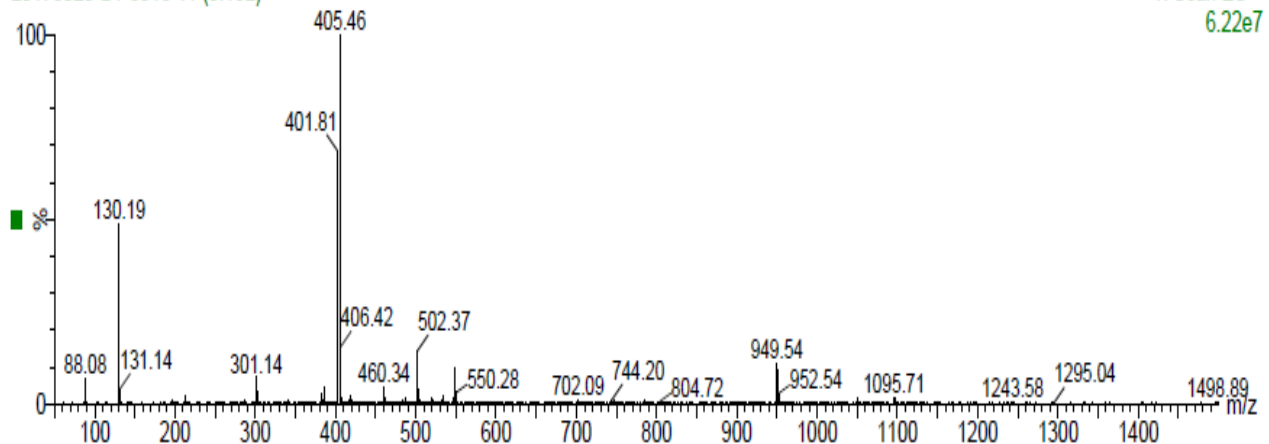

Molecular Weight:	401.97
m/z(M) Base Peak :	401.81
m/z(M+5H) Base Peak :	406.42

