

Mass Spectrometry

Analysis Information

Product Name: Digitoxin

Operator: David

Injection Date: 04/11/2024 8:34:39 PM

Inj. Volume: 1

Batch No.: 2

Acquisition Parameter

Probe: ESI

Gas Temp: 350°C

Gas Flow: 11L/min

Nebulizer: 50psi

VCap: 4000v

Fragmentor: 70v

Reference: m/z 121.050873, 922.009798

T.Flow: 0.3ml/min


B.conc: 20%H₂O/80%ACN

Result

NT-S20240411-085

20240411-71-63-6 7 (0.360)

2: Scan ES-
5.97e5

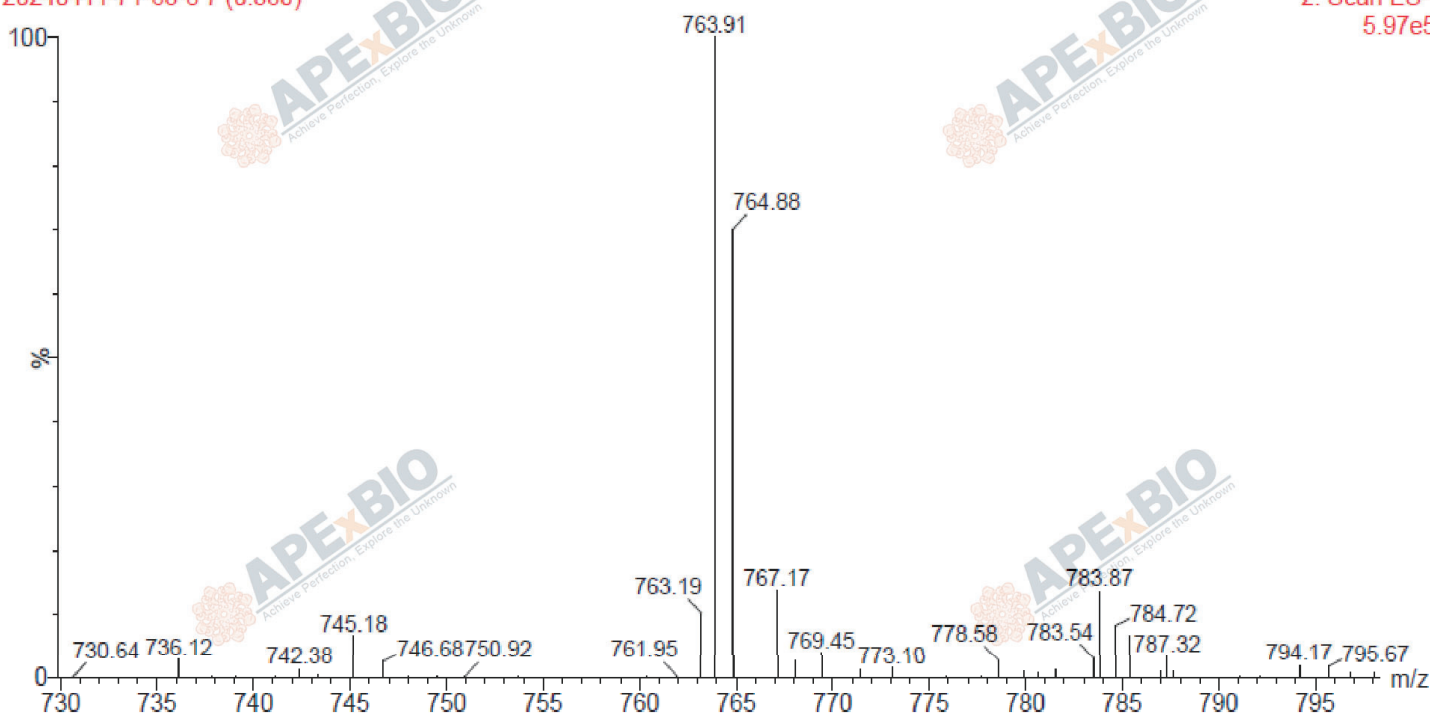

Molecular Weight: 764.95

m/z([M-H]-) Base Peak: 763.91

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

