

High Performance Liquid Chromatography

1. Analysis Information

Product Name:	SR9011
Operator:	David
Injection Date:	6/5/2018 3:04:29 PM
Batch No.:	2


2. HPLC Condition

Column: Athena C18, 3 μ m, 2.1mm \times 100 mm
 Solvent A: 0.1% H₃PO₄ in 100% Acetonitrile
 Solvent B: 0.1% H₃PO₄ in 100% Water

Gradient:	Time	A	B
	0.0min	0%	100%
	2.0min	0%	100%
	7.0min	95%	5%
	10.0min	95%	5%
	10.0min	Stop	Stop

Flow rate: 0.45ml/min
 Wavelength: 210nm
 Volume: 10 μ l

3. Result

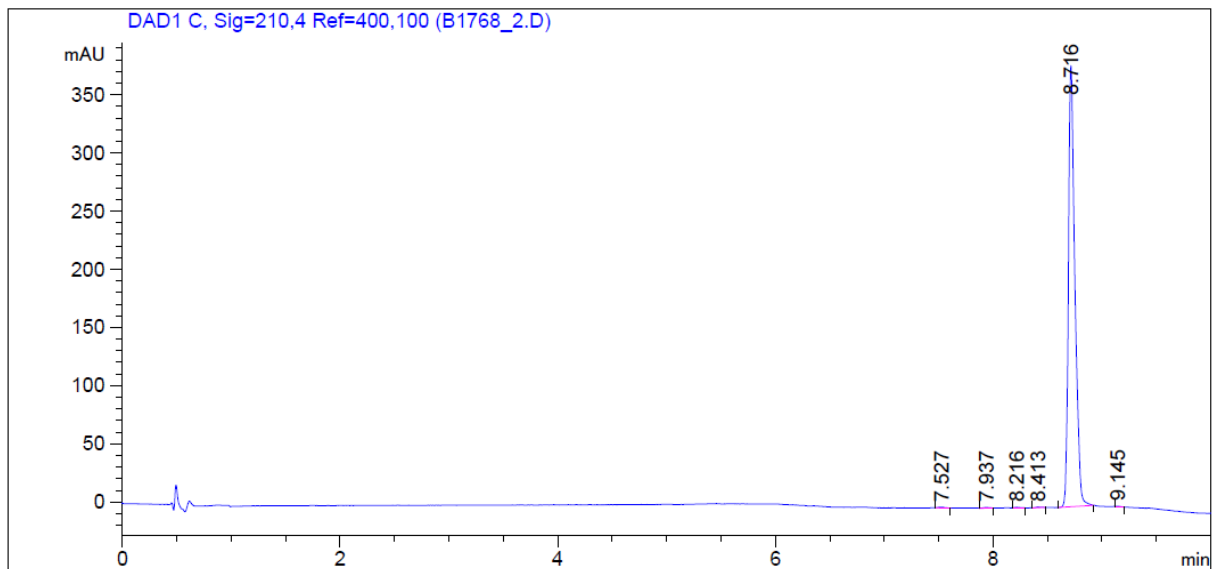

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.527	3.34551	0.2124
2	7.937	2.20254	0.1399
3	8.216	1.96439	0.1247
4	8.413	2.29904	0.1460
5	8.716	1563.40295	99.2718
6	9.145	1.65654	0.1052