



High Performance Liquid Chromatography


1. Analysis Information

Product Name:	BAY 80-6946 (Copanlisib)
Operator:	David
Injection Date:	7/15/2016 5:53:48 PM
Batch No.:	1

2. HPLC Condition

Column:	Athena C18, 3 μ m, 2.1mm \times 100 mm																			
Solvent A:	0.1% H3PO4 in 100% Acetonitrile																			
Solvent B:	0.1% H3PO4 in 100% Water																			
Gradient:	<table border="1"><thead><tr><th>Time</th><th>A</th><th>B</th></tr></thead><tbody><tr><td>0.0min</td><td>0%</td><td>100%</td></tr><tr><td>2.0min</td><td>0%</td><td>100%</td></tr><tr><td>7.0min</td><td>95%</td><td>5%</td></tr><tr><td>10.0min</td><td>95%</td><td>5%</td></tr><tr><td>10.0min</td><td>Stop</td><td>Stop</td></tr></tbody></table>		Time	A	B	0.0min	0%	100%	2.0min	0%	100%	7.0min	95%	5%	10.0min	95%	5%	10.0min	Stop	Stop
Time	A	B																		
0.0min	0%	100%																		
2.0min	0%	100%																		
7.0min	95%	5%																		
10.0min	95%	5%																		
10.0min	Stop	Stop																		
Flow rate:	0.5ml/min																			
Wavelength:	280nm																			
Volume:	3.0 μ l																			

3. Result

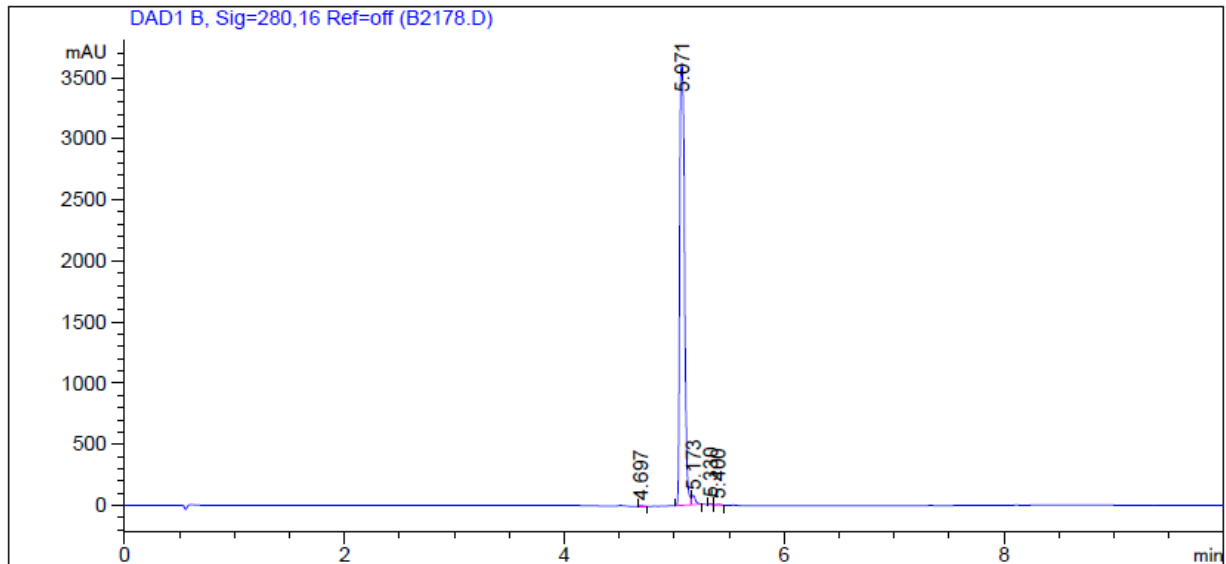

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.697	10.47926	0.0934
2	5.071	1.10064e4	98.1361
3	5.173	169.08125	1.5076
4	5.330	13.05743	0.1164
5	5.400	16.42943	0.1465