

High Performance Liquid Chromatography

Analysis Information

Product Name: FLI-06
Operator: David
Injection Date: 5/14/2019 10:21:43 PM
Batch No.: 1

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.00min	0%	100%
12.00min	0%	100%
12.10min	80%	20%
15.00min	Stop	Stop

Flow rate: 1mL/min

Wavelength: 280nm

Volume: 3 μ l

Result

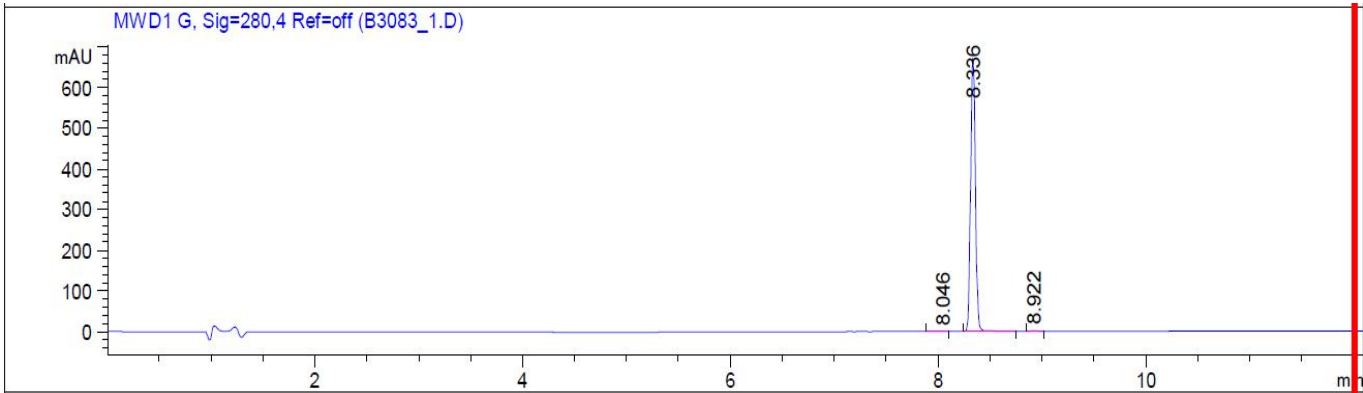

Rank	RetTime(min)	Area(mAU*s)	Area %
1	8.046	2.41427	0.1108
2	8.336	2174.94238	99.7865
3	8.922	2.23901	0.1027

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com