

High Performance Liquid Chromatography

Analysis Information

Product Name: MSDC-0160

Operator: David

Injection Date: 6/10/2020 8:45:18 AM

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 5 μ l

Result

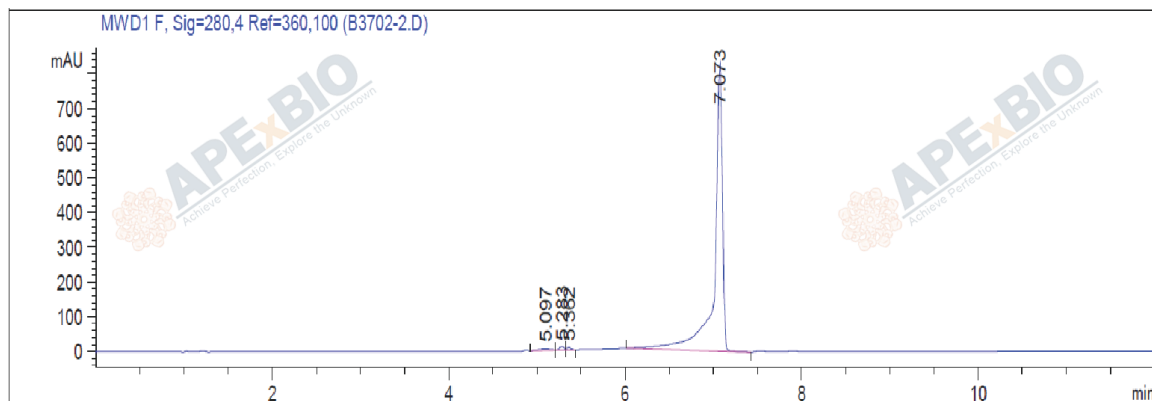

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.097	63.00069	1.1577
2	5.283	42.98943	0.7900
3	5.362	25.06158	0.4605
4	7.073	5310.71533	97.5917

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com