

High Performance Liquid Chromatography

Analysis Information

Product Name: BAPTA-AM

Operator: David

Injection Date: 4/21/2022 13:27:26 PM

Batch No.: 3

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 254nm

Volume: 20 μ l

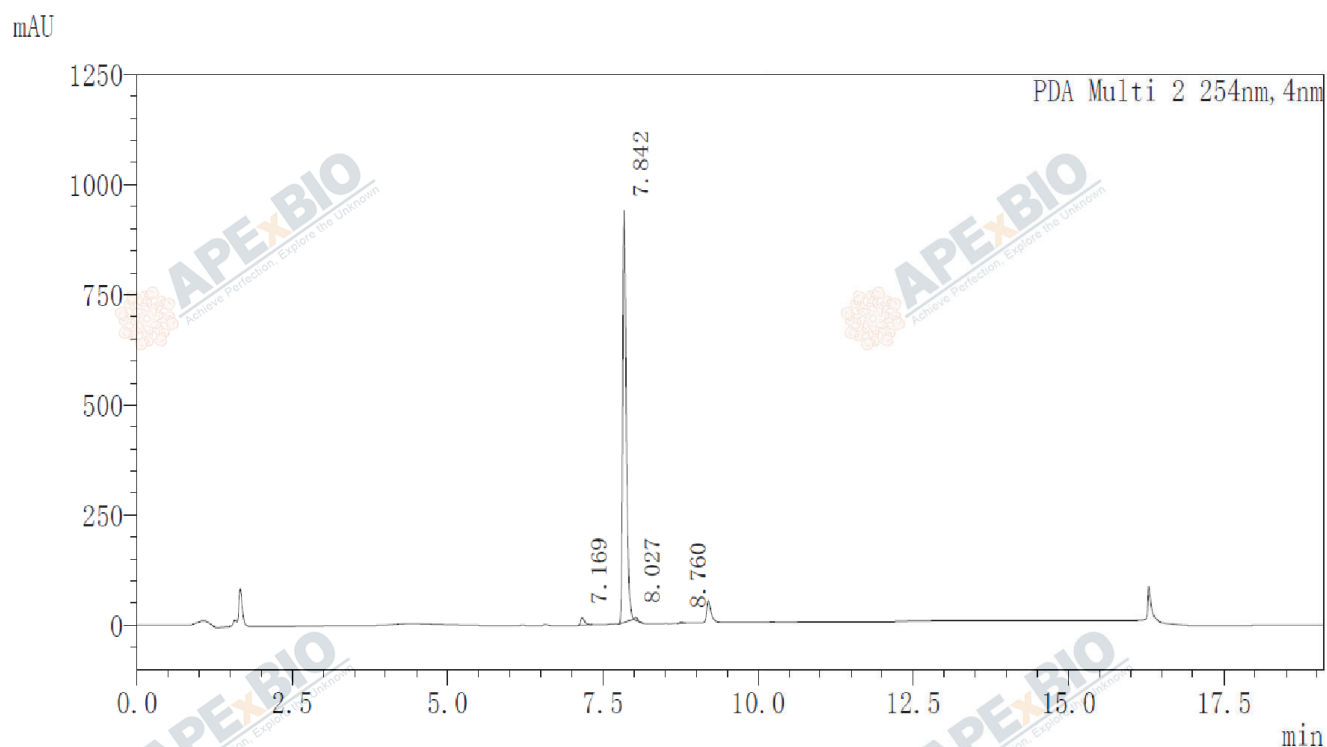

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.169	79244	2.014
2	7.842	3826569	97.242
3	8.027	18902	0.480
4	8.760	10402	0.264

Caution**FOR RESEARCH PURPOSES ONLY.****NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.****APEX BIO Technology****www.apexbt.com**

7505 Fannin street, Suite 410, Houston, TX 77054.

