

# High Performance Liquid Chromatography


## 1. Analysis Information

Product Name:	GKT137831
Operator:	David
Injection Date:	5/16/2017 11:48:16 PM
Batch No.:	2

## 2. HPLC Condition

Column:	Athena C18, 3 $\mu$ m, 2.1mm $\times$ 100 mm																			
Solvent A:	0.1% H <sub>3</sub> PO <sub>4</sub> in 100% Acetonitrile																			
Solvent B:	0.1% H <sub>3</sub> PO <sub>4</sub> in 100% Water																			
Gradient:	<table border="1"> <thead> <tr> <th>Time</th> <th>A</th> <th>B</th> </tr> </thead> <tbody> <tr> <td>0.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>2.0min</td> <td>0%</td> <td>100%</td> </tr> <tr> <td>7.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>95%</td> <td>5%</td> </tr> <tr> <td>10.0min</td> <td>Stop</td> <td>Stop</td> </tr> </tbody> </table>		Time	A	B	0.0min	0%	100%	2.0min	0%	100%	7.0min	95%	5%	10.0min	95%	5%	10.0min	Stop	Stop
Time	A	B																		
0.0min	0%	100%																		
2.0min	0%	100%																		
7.0min	95%	5%																		
10.0min	95%	5%																		
10.0min	Stop	Stop																		
Flow rate:	0.45ml/min																			
Wavelength:	254nm																			
Volume:	10 $\mu$ l																			

## 3. Result

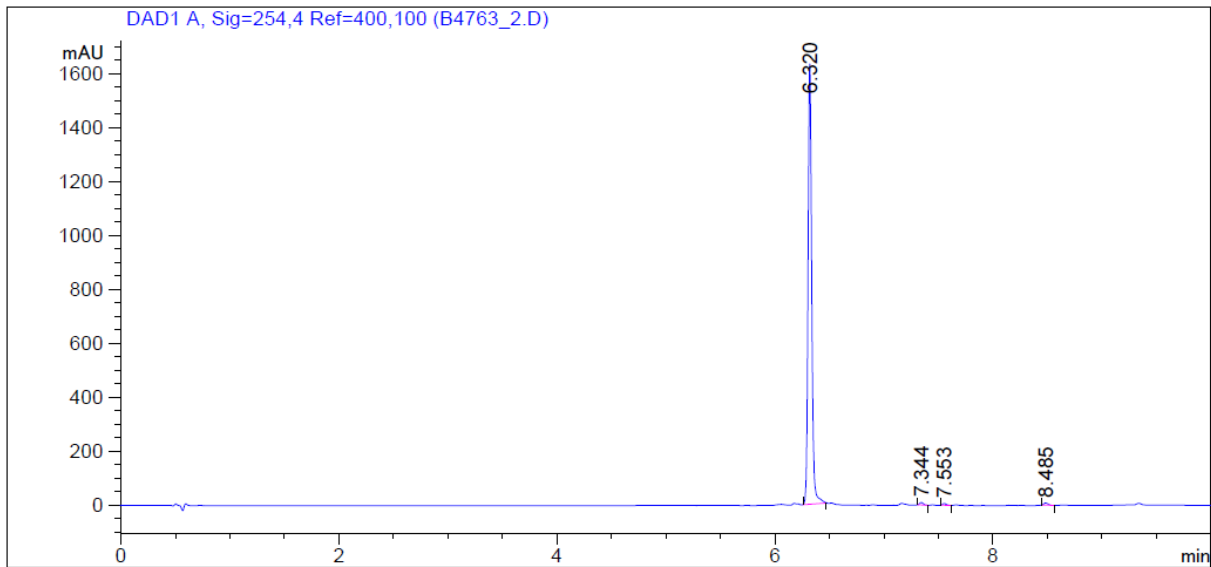

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.320	3825.16699	98.5431
2	7.344	20.47393	0.5274
3	7.553	14.35409	0.3698
4	8.485	21.72459	0.5597