

High Performance Liquid Chromatography

Analysis Information

Product Name: DTP3 TFA

Operator: David

Injection Date: 12/24/2021 10:56:02 AM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 210nm

Volume: 3 μ l

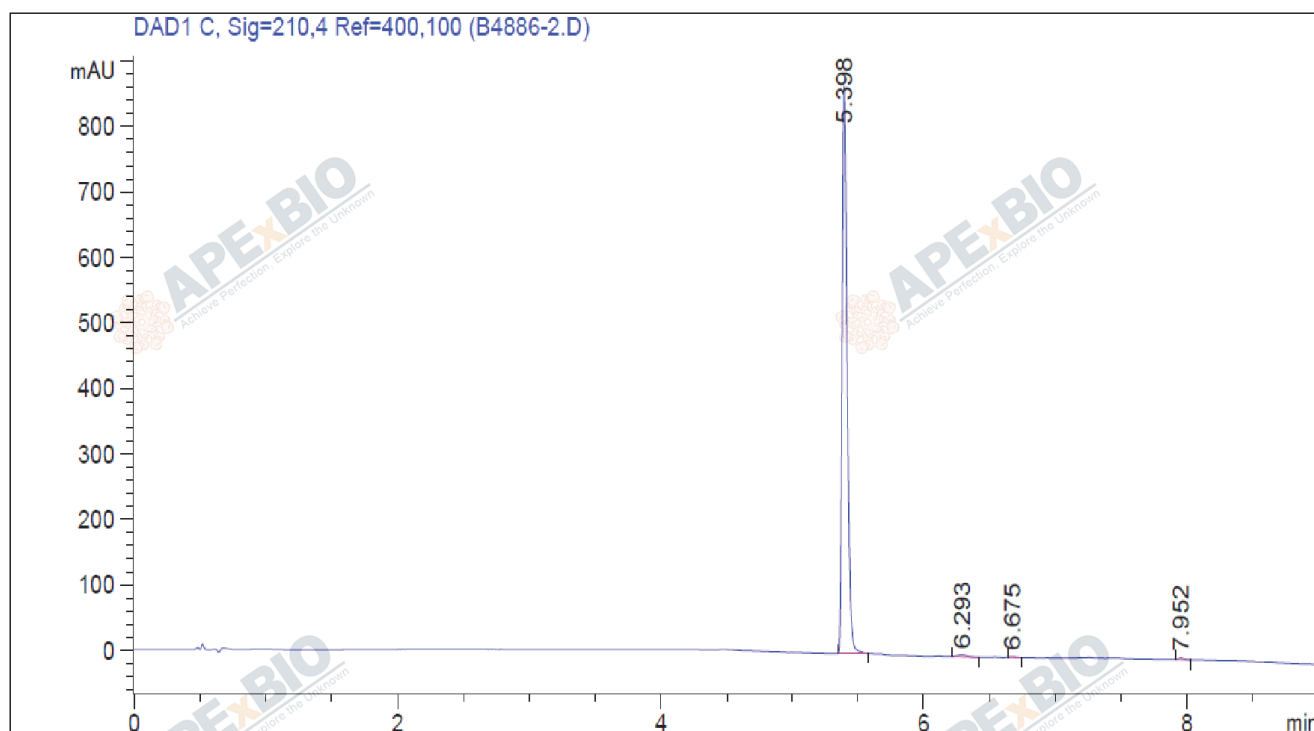

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.398	2329.43896	98.9883
2	6.293	13.40052	0.5694
3	6.675	3.37678	0.1435
4	7.952	7.03012	0.2987

Caution**FOR RESEARCH PURPOSES ONLY.****NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.****APExBIO Technology****www.apexbt.com**

7505 Fannin street, Suite 410, Houston, TX 77054.

