

High Performance Liquid Chromatography

Analysis Information

Product Name: CVT 10216

Operator: David

Injection Date: 3/4/2022 2:04:45 PM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA

Gradient:


Time	A	B
0.0min	10%	90%
5.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 254nm

Volume: 3 μ l

Result

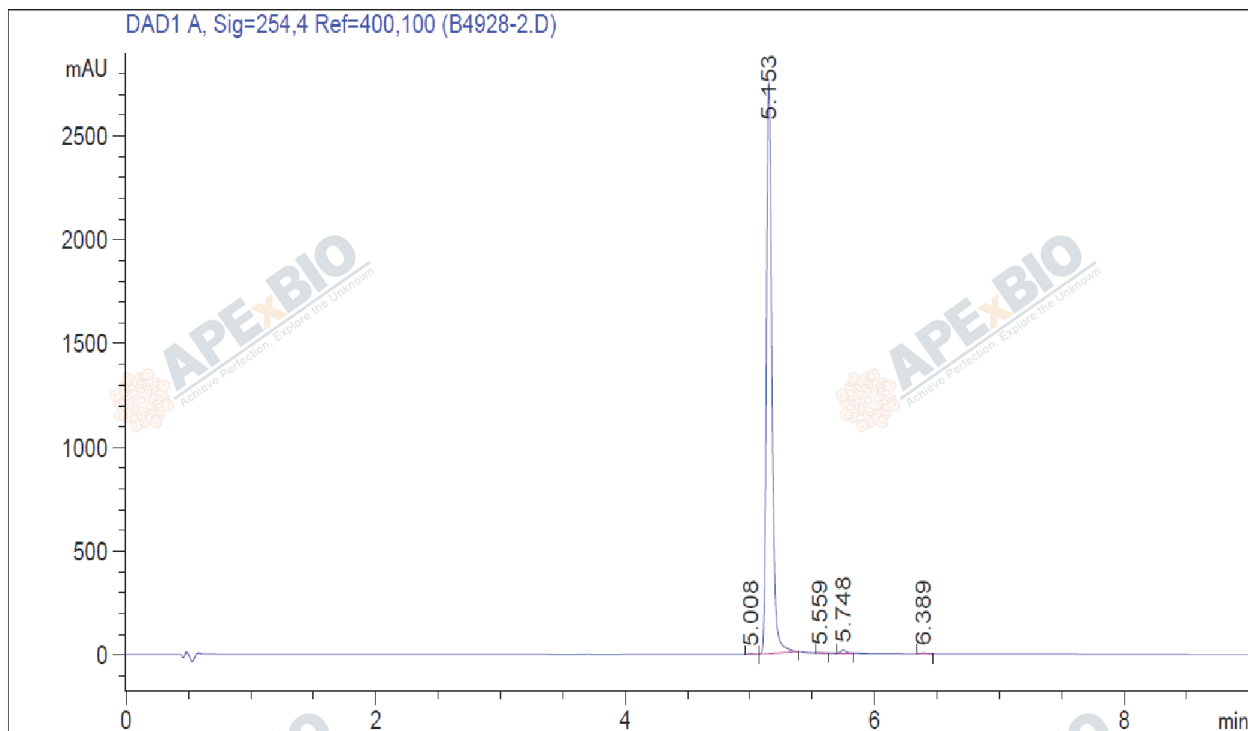

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.008	10.14344	0.1187
2	5.153	8472.61426	99.1353
3	5.559	4.08833	0.0478
4	5.748	46.78021	0.5474
5	6.389	12.89081	0.1508

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

