

High Performance Liquid Chromatography

Analysis Information

Product Name: ES 936

Operator: David

Injection Date: 5/26/2022 12:21:35 AM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 220nm

Volume: 1 μ l

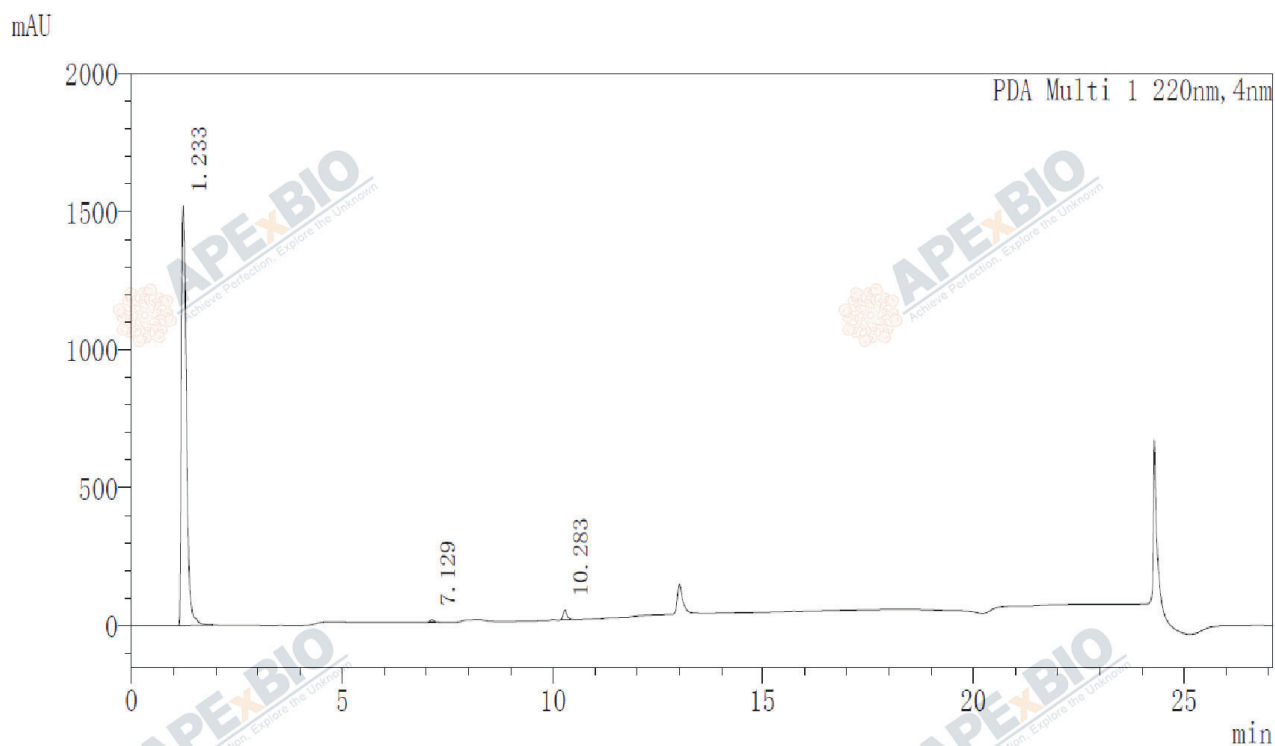

Rank	RetTime(min)	Area(mAU*s)	Area %
1	1.233	12618316	98.122
2	7.129	48630	0.378
3	10.283	192819	1.499

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com

