

Mass Spectrometry

Analysis Information

Product Name: SIB 1553A hydrochloride
Operator: David
Injection Date: 8/5/2019 5:19:08 PM
Inj. Volume: 1
Batch No.: 2

Acquisition Parameter


Probe: ESI
Gas Temp: 350°C
Gas Flow: 11L/min
Nebulizer: 50psi
VCap: 4000v
Fragmentor: 70v
Reference: m/z 121.050873, 922.009798
T.Flow: 0.3ml/min
B.conc: 20%H₂O/80%ACN

Result

NT-S20190802-081

20190805-191611-89-9 10 (0.165)

1: Scan ES+
8.86e7

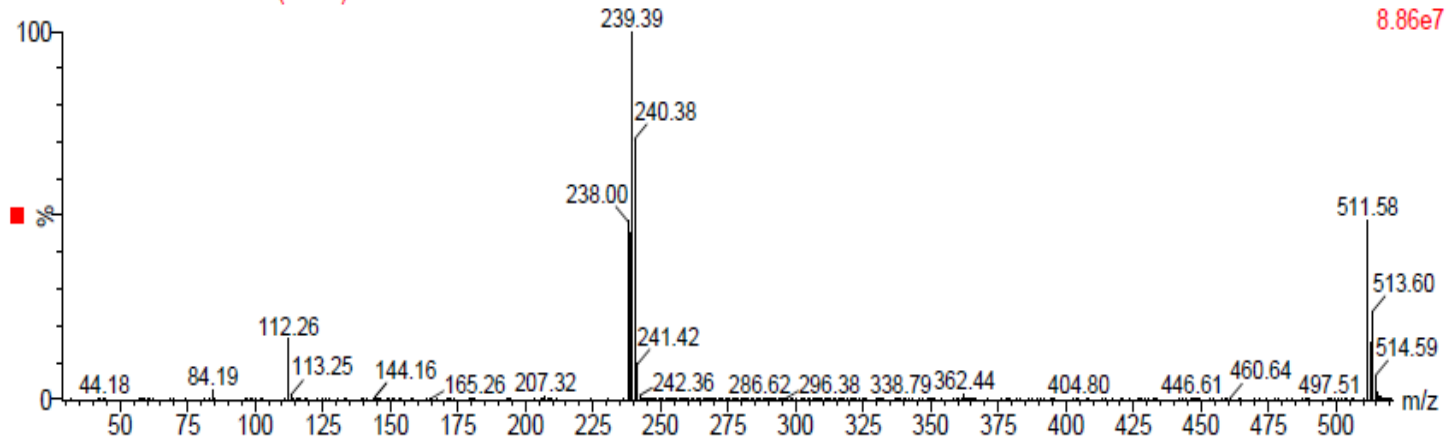

Molecular Weight: 273.82

m/z([M-HCl+3H]-) Base Peak: 239.39

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com