

High Performance Liquid Chromatography

Analysis Information

Product Name: Methoxy-X04

Operator: David

Injection Date: 8/28/2023 15:09:19

Batch No.: 3

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 265nm

Volume: 2 μ l

Result

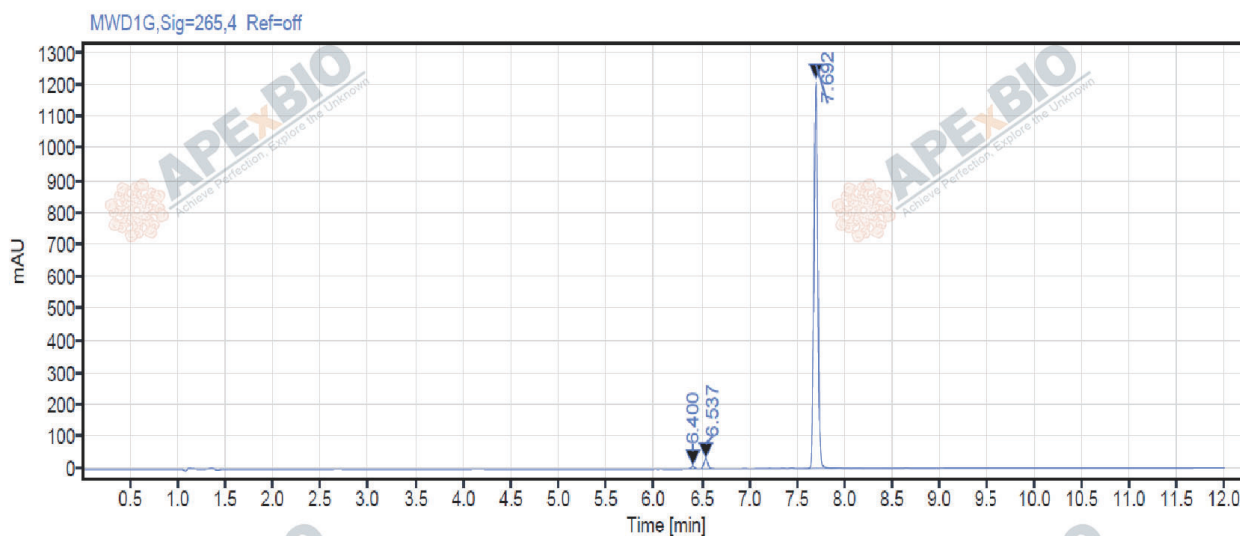

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.400	26.12	0.72
2	6.537	95.02	2.61
3	7.692	3516.87	96.67

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com