

Mass Spectrometry

Analysis Information


Product Name:	BPTES
Operator:	David
Injection Date:	3/4/2019 11:44:39 AM
Inj. Volume:	1
Batch No.:	2

Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

Result

Sample Name	0304	Position	P2-A1	Instrument Name	Instrument 1
User Name		Inj Vol	Unknown / Injection Program	InjPosition	
Sample Type	Sample	IRM Calibration Status	Success	Data Filename	B6008-2-POS.d
ACQ Method	20190215-HPLC-POS.m	Comment		Acquired Time	3/4/2019 11:44:39 AM (UTC+08:00)

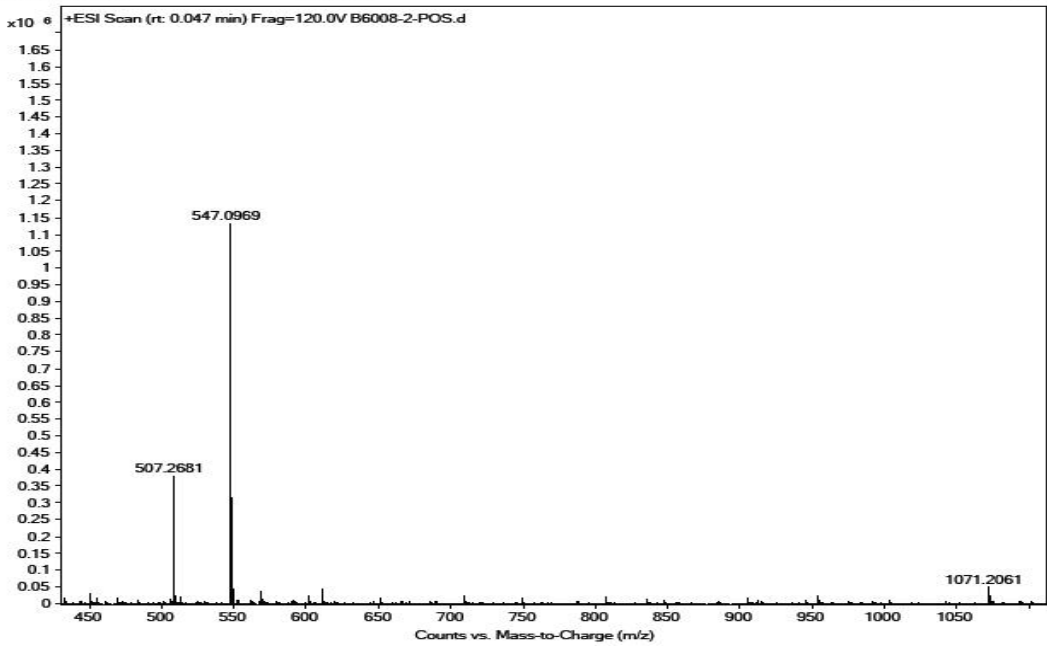

Molecular Weight: 524.68

m/z([M+Na]⁺) Base Peak: 547.0969

m/z([M-H-O]⁻) Base Peak: 507.2681

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com