

High Performance Liquid Chromatography

Analysis Information

Product Name: Cyclo(RGDyK)
Operator: David
Injection Date: 2/28/2020 1:34:16 PM
Batch No.: 3


HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm
Solvent A: H2O+1‰ TFA
Solvent B: ACN+1‰ TFA
Gradient:

Time	A	B
0.0min	95%	5%
2.0min	95%	5%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min
Wavelength: 280nm
Volume: 5 μ l

Result

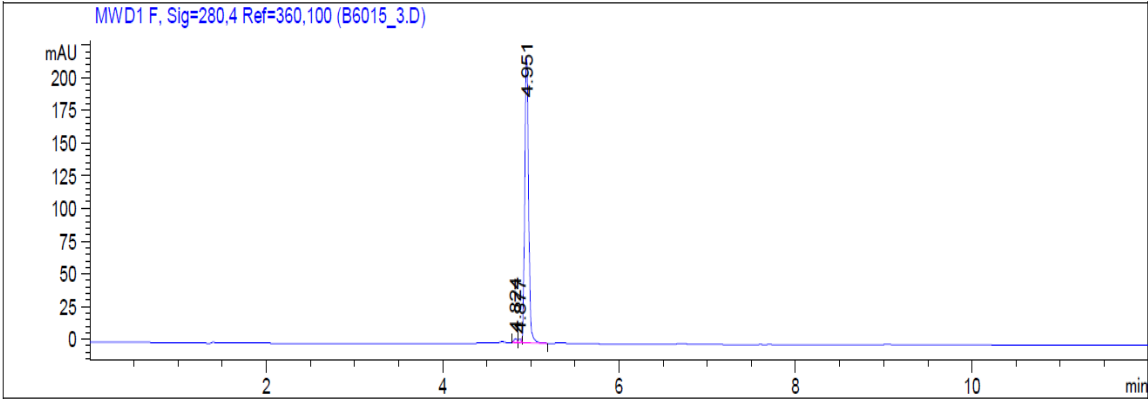

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.824	7.55900	1.1145
2	4.877	5.71163	0.8421
3	4.951	664.95758	98.0433

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com