

High Performance Liquid Chromatography

Analysis Information

Product Name: RSL3

Operator: David

Injection Date: 10/15/2024 13:48:42

Batch No.: 6

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 2 μ l

Result

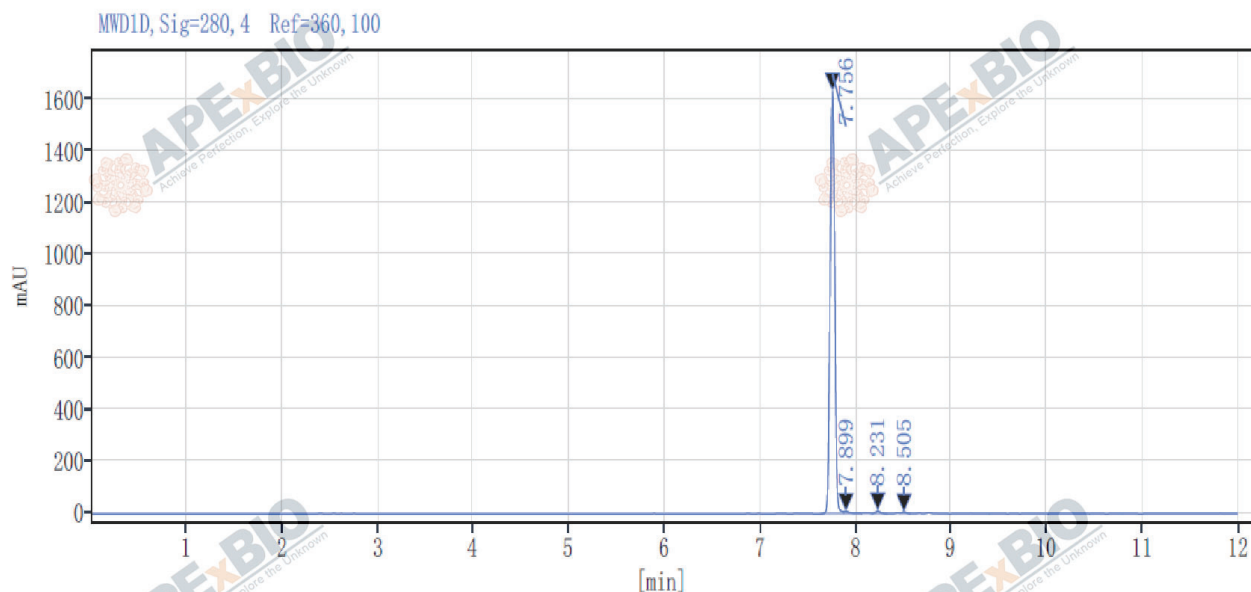

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.756	5214.34	98.44
2	7.899	32.36	0.61
3	8.231	31.84	0.60
4	8.505	18.40	0.35

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

