

High Performance Liquid Chromatography

Analysis Information

Product Name: FRAX486
Operator: David
Injection Date: 1/21/2019 12:02:25 PM
Batch No.: 2


HPLC Condition

Column : Athena C18 3 μ m 2.1mmx100mm
Solvent A: ACN
Solvent B: acid-1/H2O
Gradient:

| Time | A | B |
|---------|------|-------|
| 0.0min | 0% | 100% |
| 2.0min | 0% | 1000% |
| 7.0min | 95% | 5% |
| 10.0min | 95% | 5% |
| 12.0min | 0% | 100% |
| 12.1min | 80% | 20% |
| 15.0min | Stop | Stop |

Flow rate: 0.45ml/min
Wavelength: 365nm
Volume: 5 μ l

Result

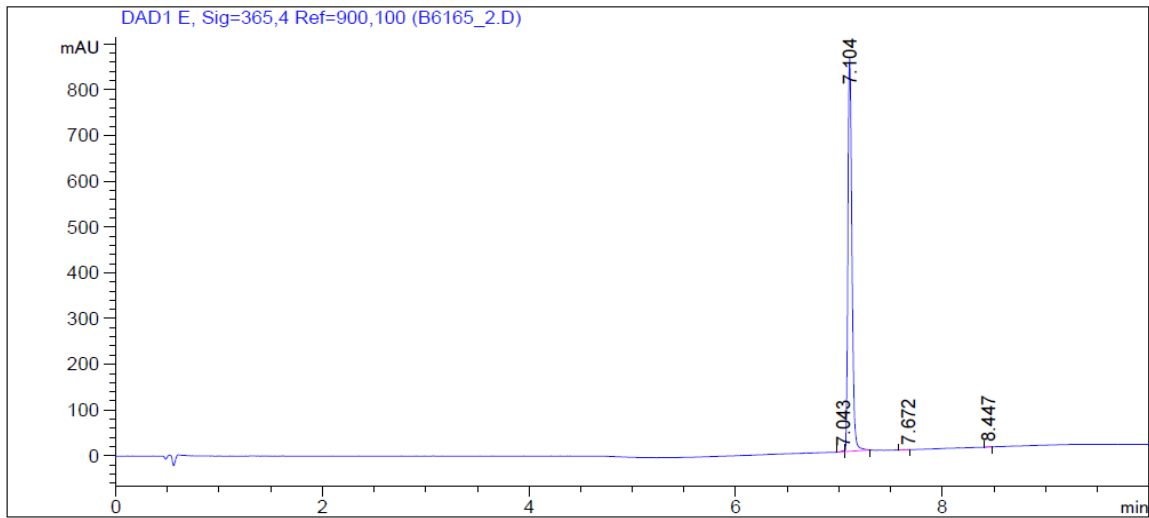

| Rank | RetTime(min) | Area(mAU*s) | Area % |
|------|--------------|-------------|---------|
| 1 | 7.043 | 4.40833 | 0.1889 |
| 2 | 7.104 | 2326.40845 | 99.7057 |
| 3 | 7.672 | 1.12354 | 0.0482 |
| 4 | 8.447 | 1.33394 | 0.0572 |

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com