

High Performance Liquid Chromatography

Analysis Information

Product Name: Rottlerin

Operator: David

Injection Date: 4/20/2023 14:45:57

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA

Gradient:


Time	A	B
0.0min	25%	75%
5min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 3 μ l

Result

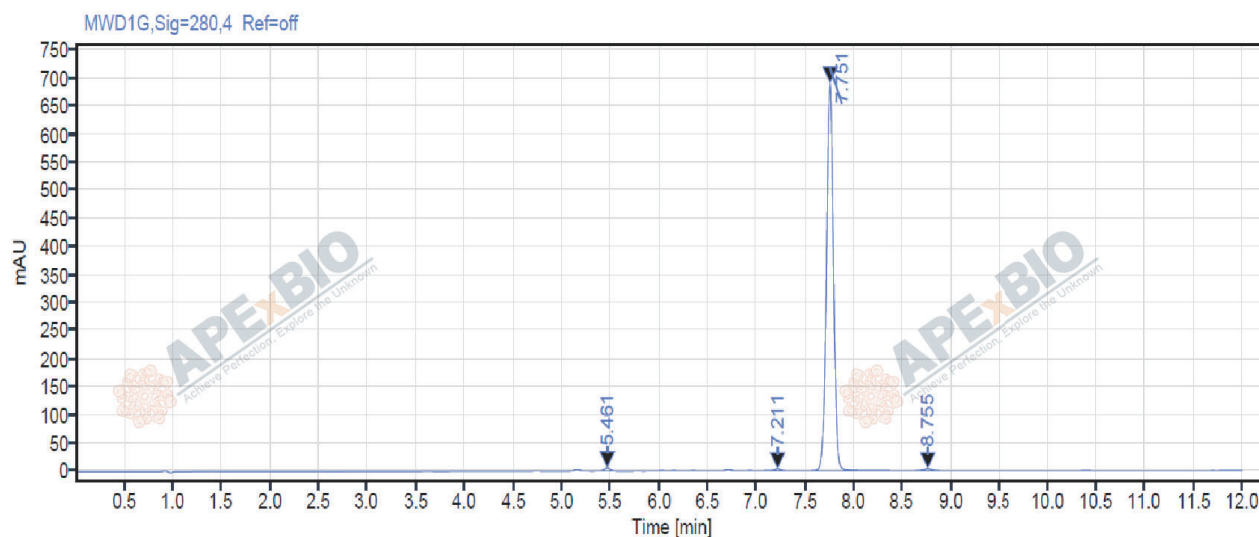

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.461	24.07	0.69
2	7.211	14.31	0.41
3	7.751	3437.08	98.30
4	8.755	21.14	0.60

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com