

High Performance Liquid Chromatography

Analysis Information

Product Name: Pseudo-UTP

Operator: David

Injection Date: 04/28/2024 21:04:29

Batch No.: 65

HPLC Condition

Column : Boston, 3 μ m, 4.6mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA

Gradient:


Time	A	B
0.0min	0%	100%
2.0min	0%	100%
7.0min	95%	5%
10.0min	95%	5%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 254nm

Volume: 10 μ l

mAU

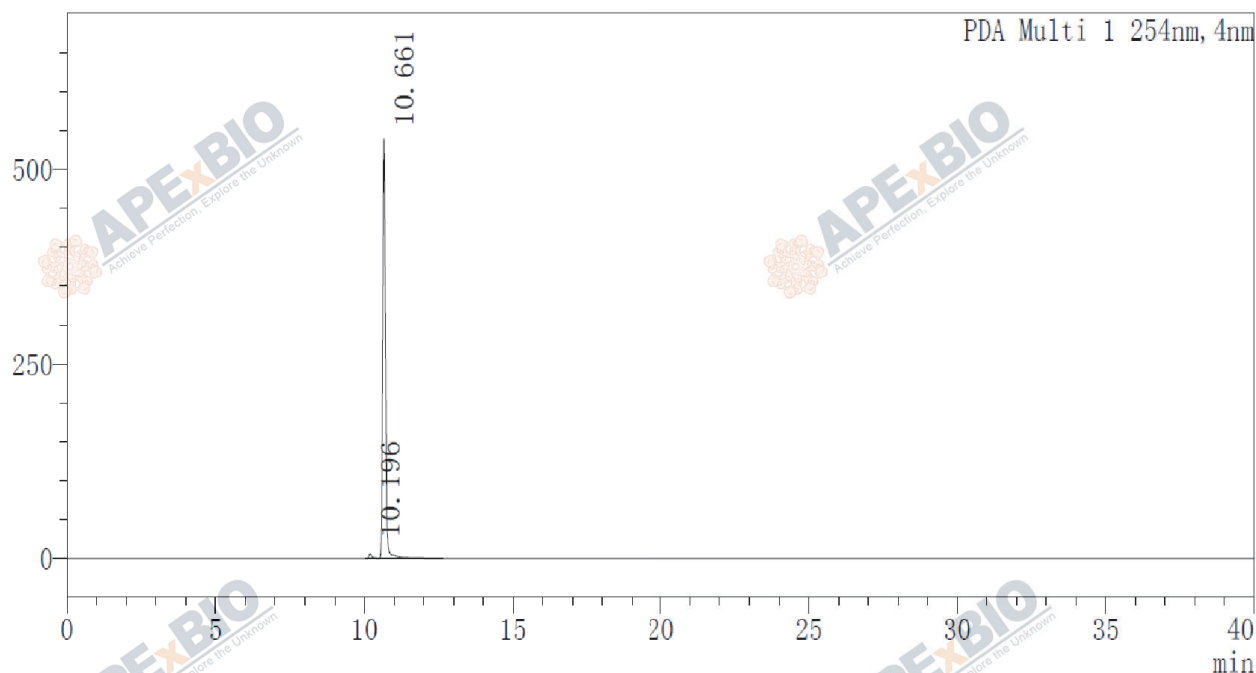

Rank	RetTime(min)	Area(mAU*s)	Area %
1	10.196	45203	1.261
2	10.661	3540590	98.739

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com