

Mass Spectrometry

Analysis Information

Product Name: Fluorescein-12-dUTP

Operator: David

Injection Date: 4/25/2023 7:30:03 PM

Inj. Volume: 1

Batch No.: 3

Acquisition Parameter

Probe: ESI

Gas Temp: 350°C

Gas Flow: 11L/min

Nebulizer: 50psi

VCap: 4000v


Fragmentor: 70v

Reference: m/z 121.050873, 922.009798

T.Flow: 0.3ml/min

B.conc: 20%H₂O/80%ACN

Result

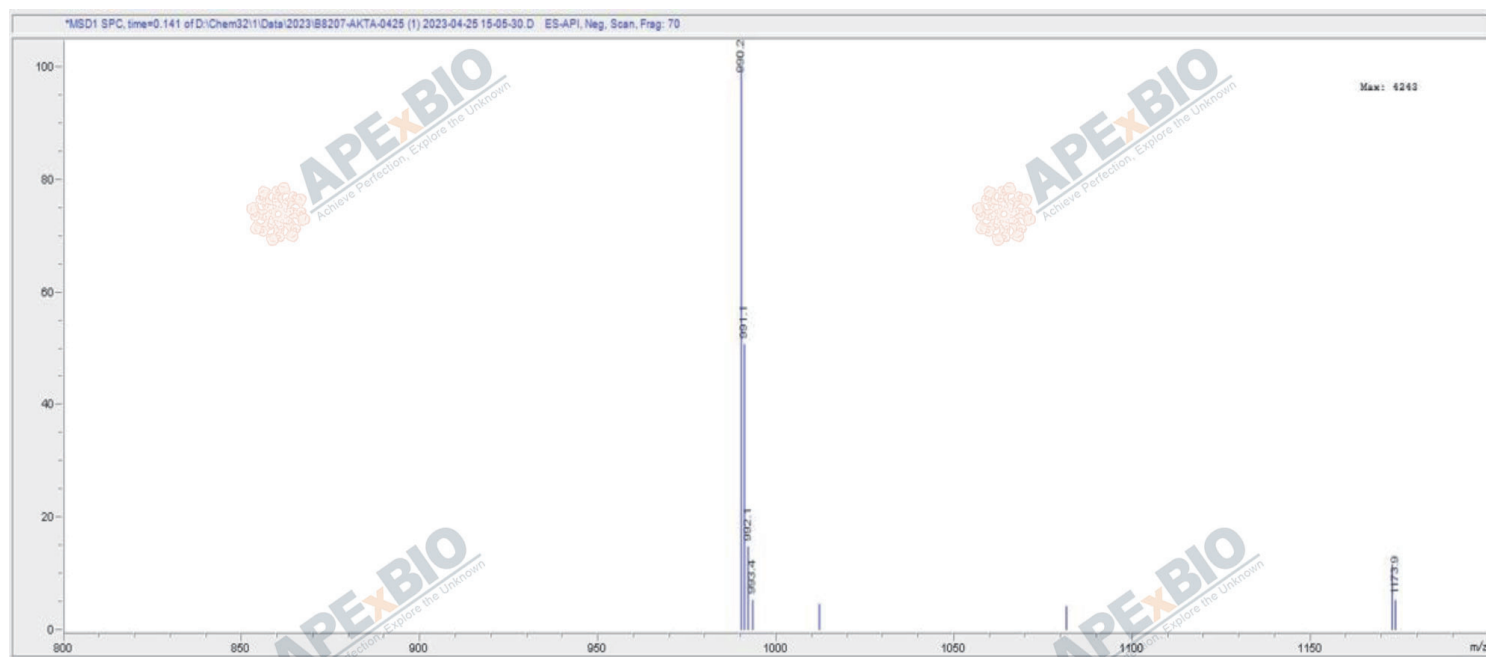

Molecular Weight: 994.69 (free acid)

m/z([M-4H]-) Base Peak: 990.2

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEXBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com