

High Performance Liquid Chromatography

Analysis Information

Product Name: ddhCTP

Operator: David

Injection Date: 5/16/2023 10:00:51 AM

Batch No.: 1

HPLC Condition

Column : Boston, 3.5 μ m, 4.6mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
2.0min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
16.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 280nm

Volume: 50 μ l

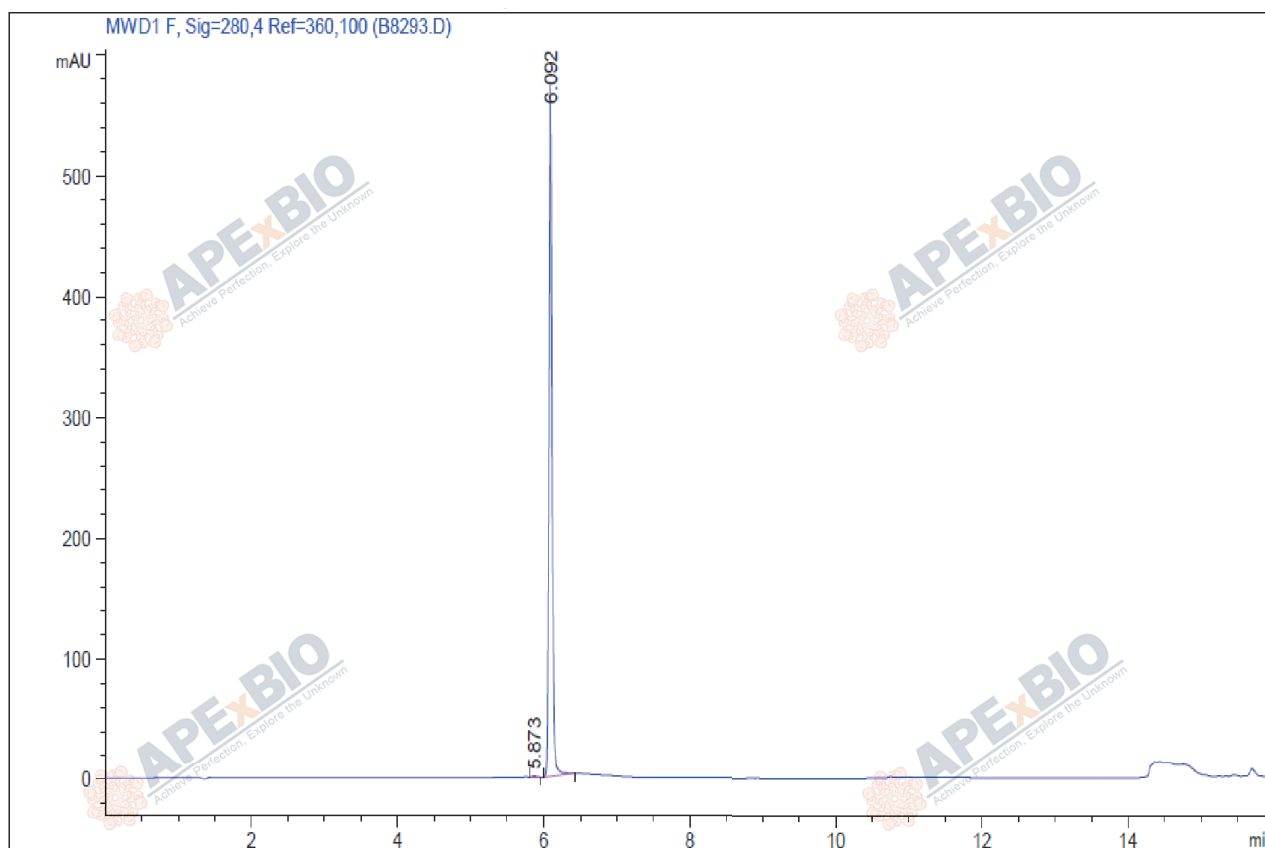

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.873	2.88993	0.1601
2	6.092	1802.14417	99.8399

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com

