

High Performance Liquid Chromatography

Analysis Information

Product Name: Golgi-Tracker Green

Operator: David

Injection Date: 10/09/2024 10:06:57

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	95%	5%
2.0min	95%	5%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 220nm

Volume: 10 μ l

Result

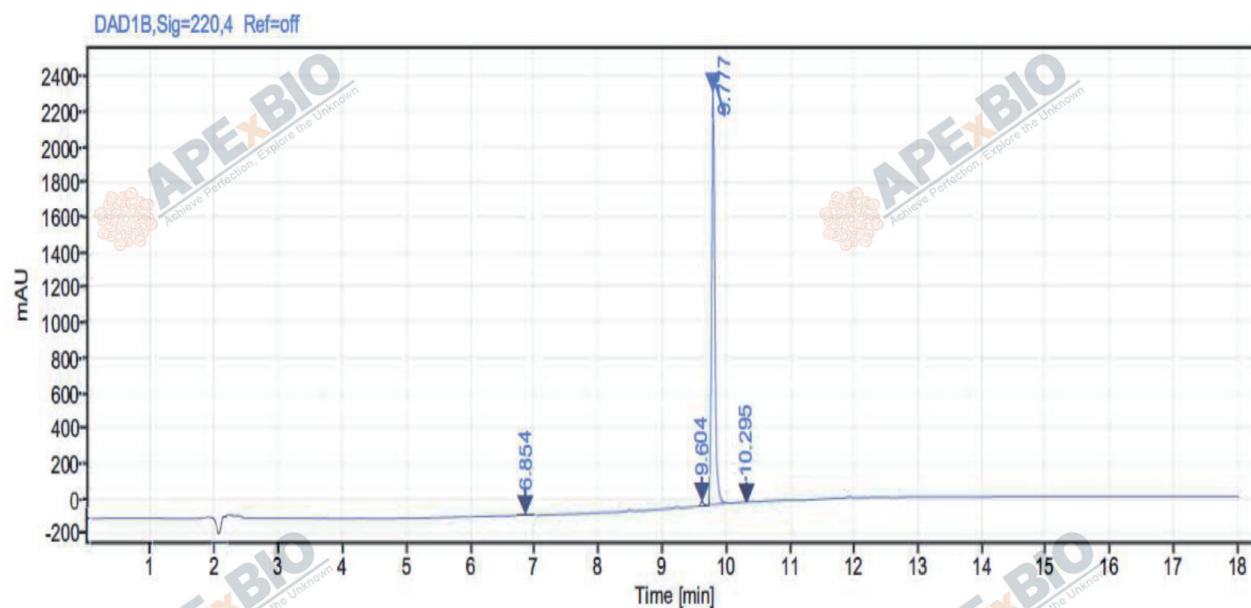

Rank	RetTime(min)	Area(mAU*s)	Area %
1	6.854	8.77	0.10
2	9.604	98.01	1.14
3	9.777	8461.32	98.62
4	10.295	11.35	0.13

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APExBIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

