

High Performance Liquid Chromatography

Analysis Information

Product Name: JD5037

Operator: David

Injection Date: 9/29/2021 4:13:59 PM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 210nm

Volume: 3 μ l

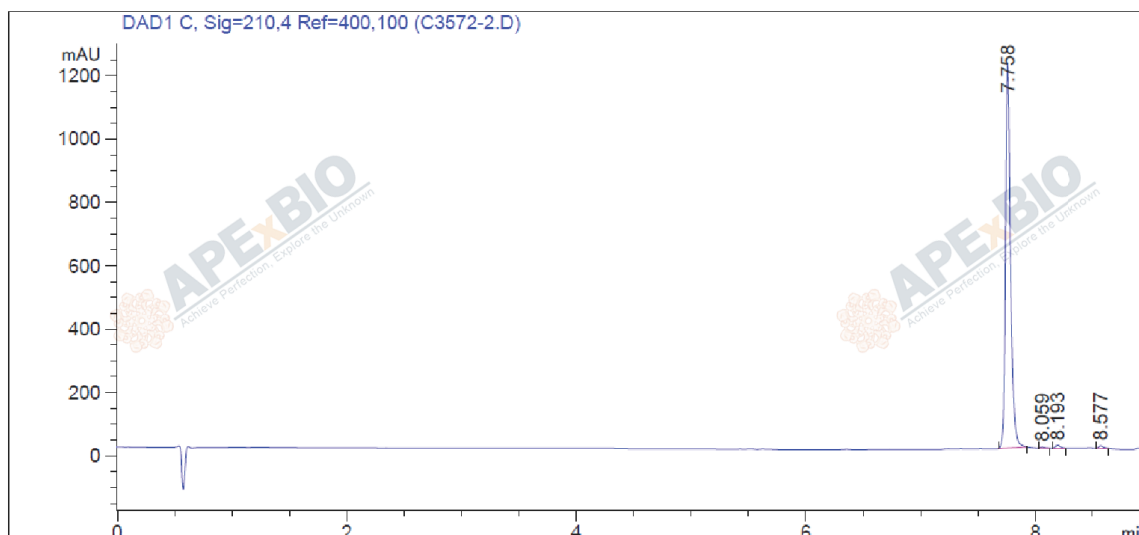

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.758	3654.49829	98.4009
2	8.059	9.11728	0.2455
3	8.193	26.83387	0.7225
4	8.577	23.43758	0.6311

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com