
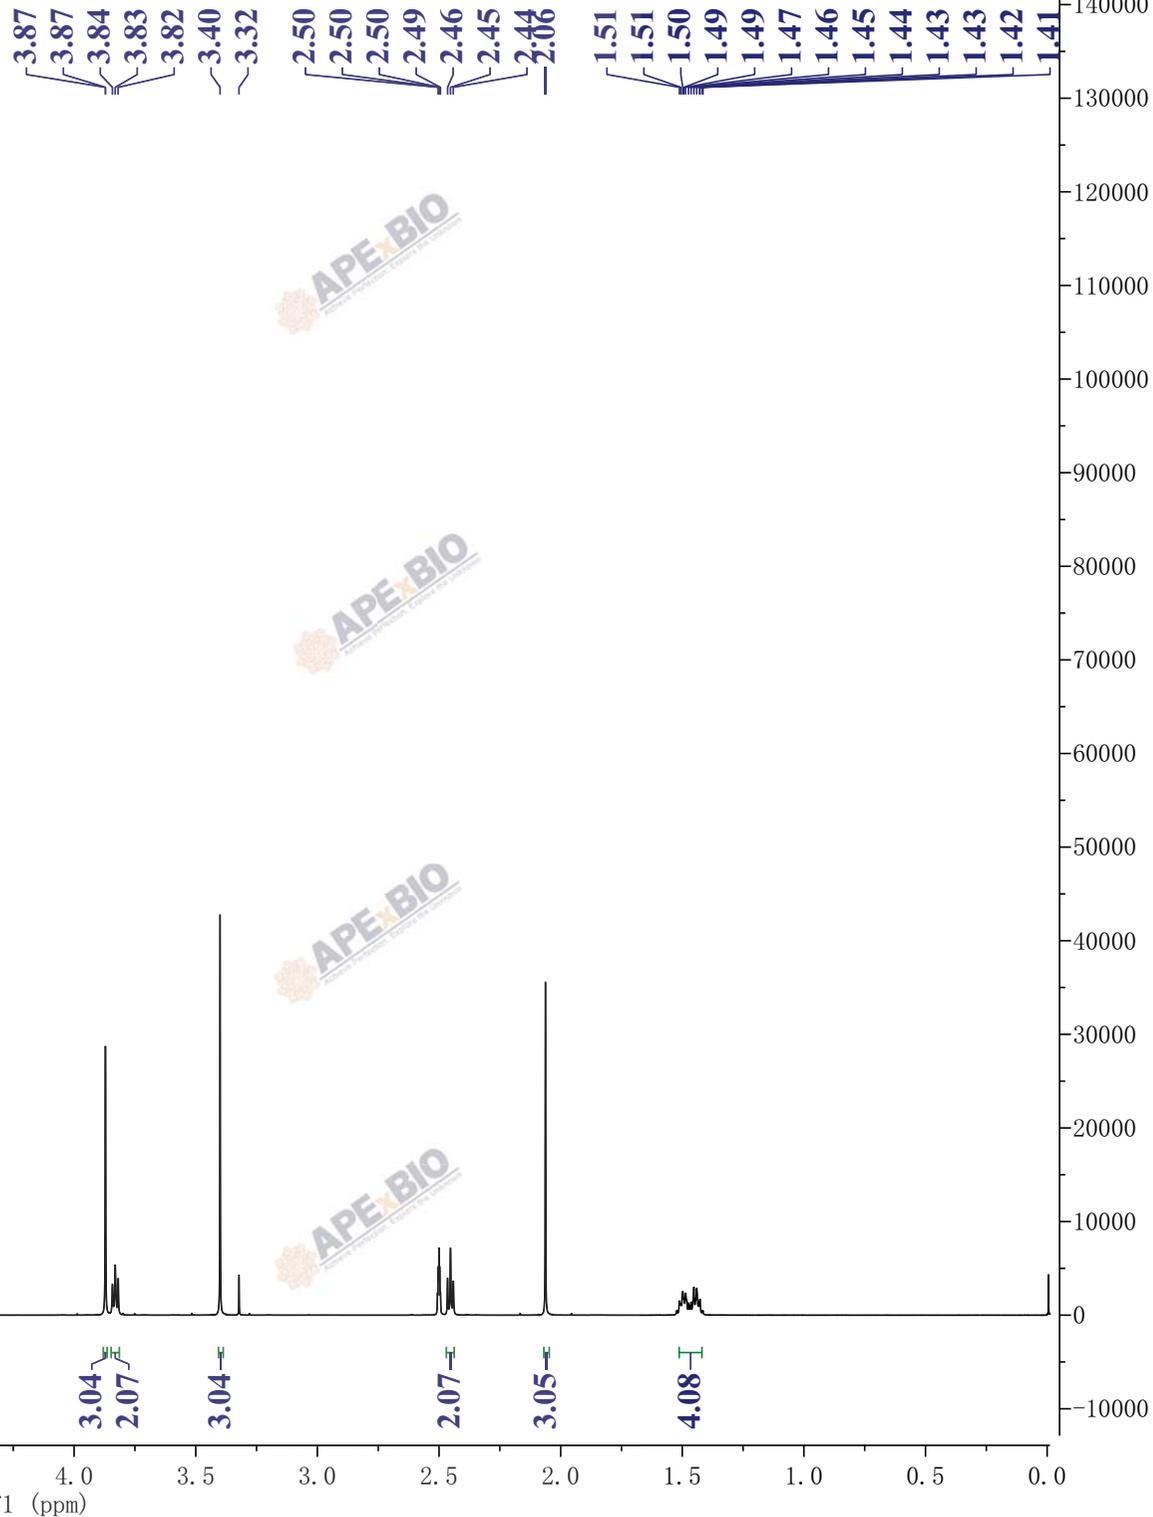


8.00
8.00

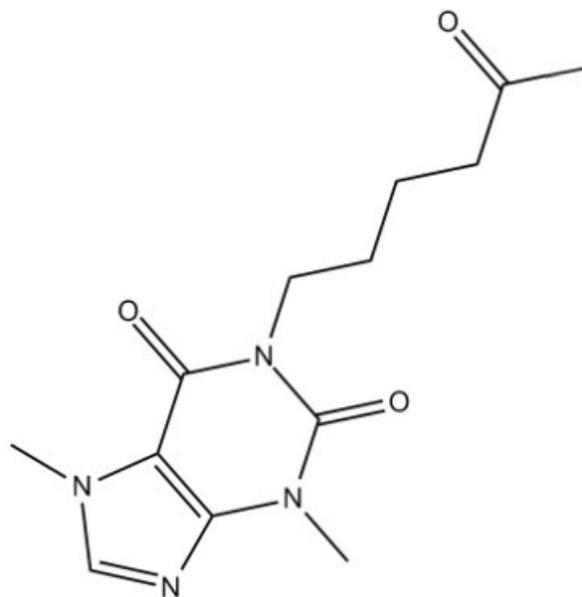

APE-BIO
ANALYTICAL LABORATORY

APE-BIO
ANALYTICAL LABORATORY