

High Performance Liquid Chromatography

Analysis Information

Product Name: WST-8

Operator: David

Injection Date: 11/16/2021 11:08:20 AM

Batch No.: 16

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 254nm

Volume: 3 μ l

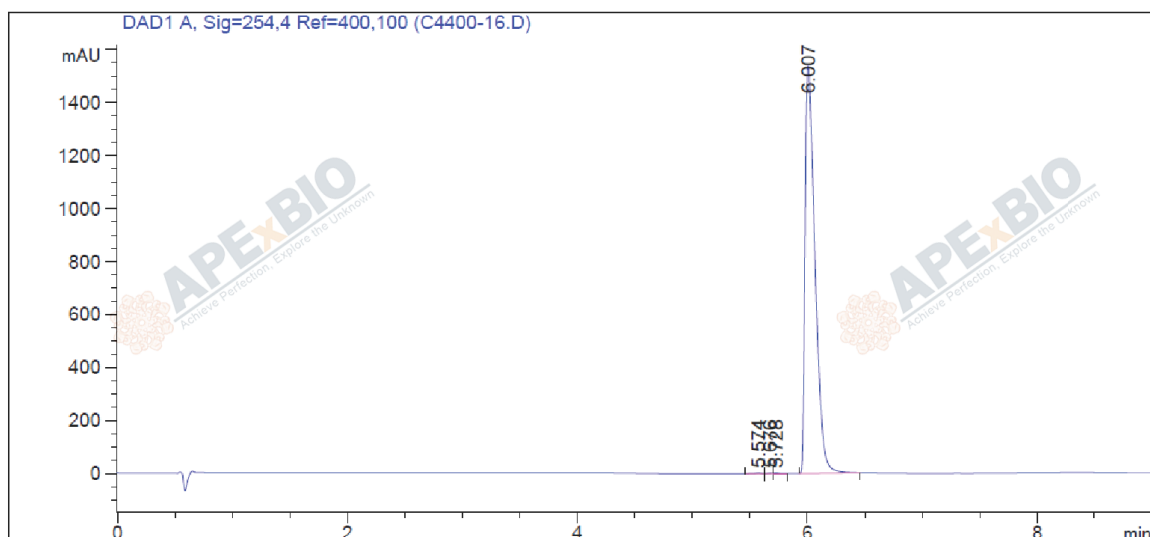

Rank	RetTime(min)	Area(mAU*s)	Area %
1	5.574	13.19603	0.1429
2	5.676	6.29552	0.0682
3	5.728	8.01841	0.0868
4	6.007	9209.10547	99.7022

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com