

High Performance Liquid Chromatography

Analysis Information

Product Name: SR9238

Operator: David

Injection Date: 02/14/2025 11:57:22

Batch No.: 2

HPLC Condition

Column : ZORBAX Eclipse Pluse C18 3.5 μ m 4.6mmx100mm

Solvent A: H2O+0.1%TFA

Solvent B: ACN+0.1%TFA

Gradient:


Time	A	B
0.0min	80%	20%
2.0min	80%	20%
7.0min	5%	95%
10.0min	0%	100%
12.0min	0%	100%
15.0min	Stop	Stop

Flow rate: 1ml/min

Wavelength: 254nm

Volume: 2 μ l

Result

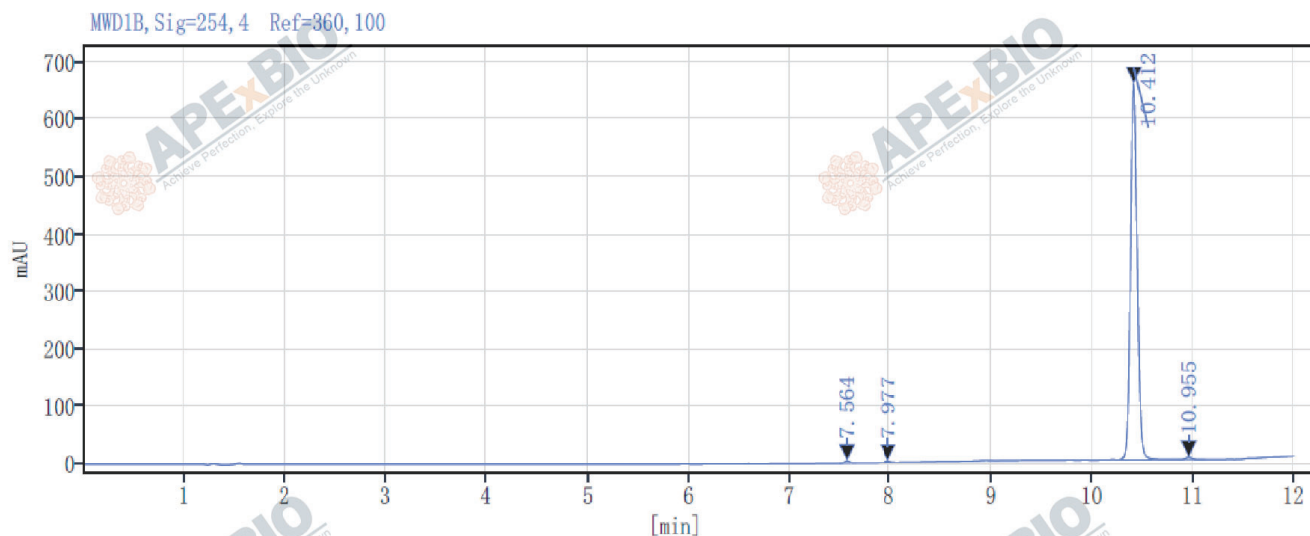

Rank	RetTime(min)	Area(mAU*s)	Area %
1	7.564	13.89	0.45
2	7.977	8.92	0.29
3	10.412	3029.90	98.65
4	10.955	18.77	0.61

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com

