

1. Analysis Information

Product Name:	Cryptochlorogenic acid
Operator:	David
Injection Date:	7/18/2017 10:12:45 PM
Inj. Volume:	1
Batch No.:	2


2. Acquisition Parameter

Probe:	ESI
Gas Temp:	350°C
Gas Flow:	11L/min
Nebulizer:	50psi
VCap:	4000v
Fragmentor:	70v
Reference:	m/z 121.050873, 922.009798
T.Flow:	0.3ml/min
B.conc:	20%H ₂ O/80%ACN

3. Result

20170718-905-99-7(1745) 11 (0.191)

2: Scan ES-
6.75e7

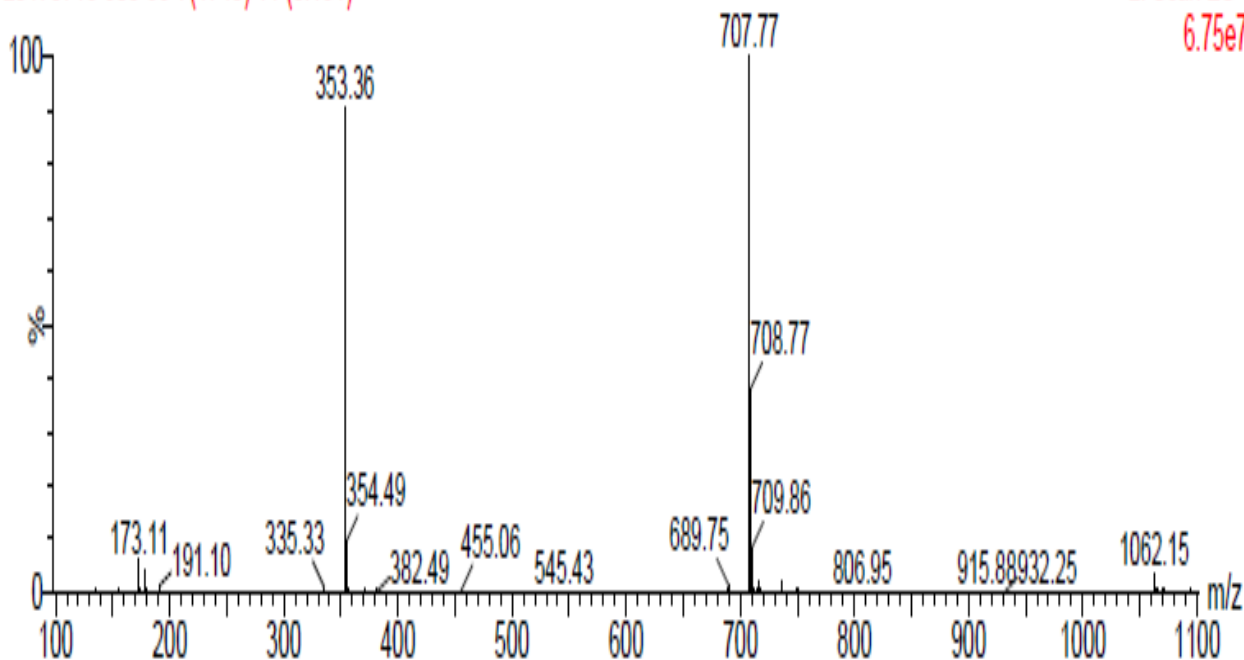

Molecular Weight:	354.31
m/z(M-H) Base Peak :	353.36
m/z(M) Base Peak :	354.49