

High Performance Liquid Chromatography

Analysis Information

Product Name: Phloridzin

Operator: David

Injection Date: 11/18/2021 8:51:09 PM

Batch No.: 2

HPLC Condition

Column : Athena C18, 3 μ m, 2.1mm $\times$ 100 mm

Solvent A: ACN+0.1%TFA

Solvent B: H2O+0.1%TFA


Gradient:

Time	A	B
0.0min	0%	100%
1.5min	0%	100%
6.0min	95%	5%
9.0min	95%	5%
9.0min	Stop	Stop

Flow rate: 0.46ml/min

Wavelength: 280nm

Volume: 3 μ l

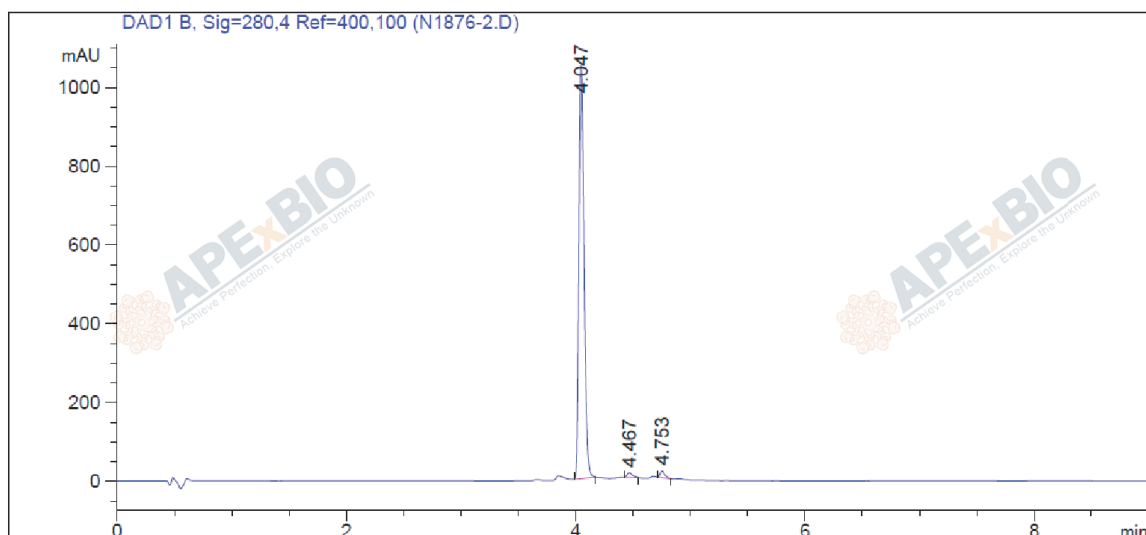

Rank	RetTime(min)	Area(mAU*s)	Area %
1	4.047	3203.29907	97.2742
2	4.467	40.56356	1.2318
3	4.753	49.19995	1.4940

Caution

FOR RESEARCH PURPOSES ONLY.

NOT FOR HUMAN, VETERINARY DIAGNOSTIC OR THERAPEUTIC USE.

APEX BIO Technology

www.apexbt.com

7505 Fannin street, Suite 410, Houston, TX 77054.

Tel: +1-832-696-8203 | Fax: +1-832-641-3177 | Email: info@apexbt.com